

# 12 LABORATORY SAMPLE PREPARATION

## 12.1 Introduction

On first impression, sample preparation may seem the most mundane aspect of an analytical protocol. However, it is critical that the analyst realize and remember that a determination is only as good as the sample preparation that has preceded it. If an aliquant taken for analysis does not represent the original sample accurately, the results of this analysis are questionable. As a general rule, the error in sampling and the sample preparation portion of an analytical procedure is considerably higher than that in the methodology itself, as illustrated in Figure 12.1.

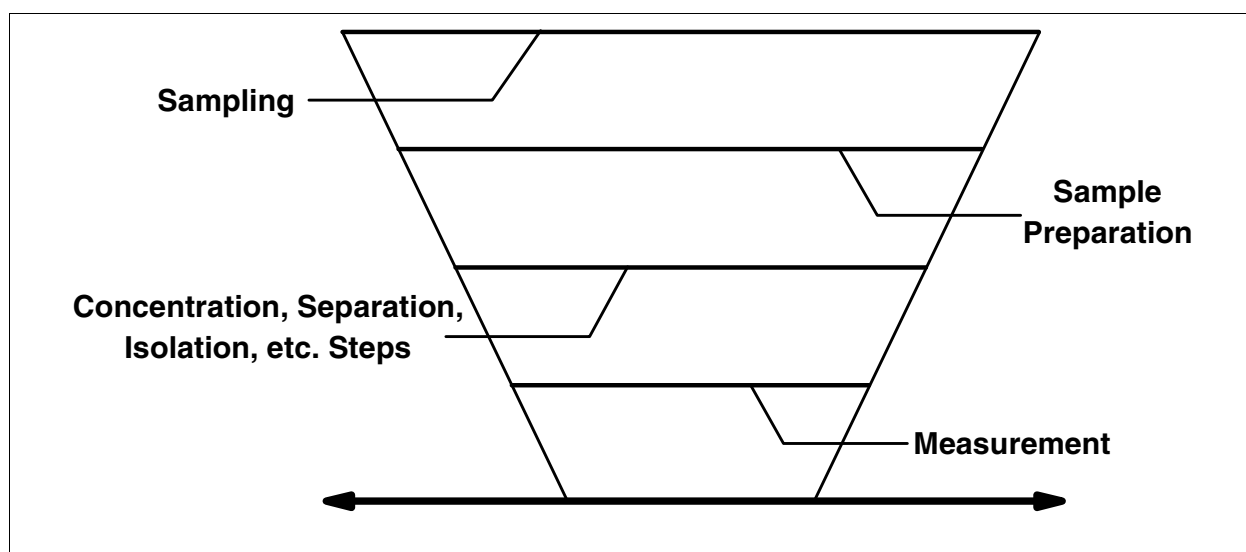


FIGURE 12.1—Degree of error in laboratory sample preparation (Scwedt, 1997)

One goal of laboratory sample preparation is to provide, without sample loss, representative aliquants that are free of laboratory contamination that will be used in the next steps of the protocol. Samples are prepared in accordance with applicable standard operating procedures (SOPs) and laboratory SOPs using information provided by field sample preparation (Chapter 10, *Field and Sampling Issues that Affect Laboratory Measurements*), sample screening activities, and objectives given in the appropriate planning documents. *The laboratory sample preparation techniques presented in this chapter include the physical manipulation of the sample (heating, screening, grinding, mixing, etc.) up to the point of dissolution. Steps such as adding carriers and tracers, followed by wet ashing or fusion, are discussed in Chapter 13 (Sample Dissolution) and Chapter 14 (Separation Techniques).*

This chapter presents some general guidance for sample preparation on the avoidance of sample loss and of sample contamination. Owing to the physical nature of the media, sample preparation for solids requires the most attention, and therefore is discussed at great length (Section 12.3). General procedures for preparing solid samples (such as drying, obtaining a constant weight, grinding, sieving, mixing, and subsampling) are discussed. Some sample preparation procedures then are presented for typical types of solid samples (e.g., soil and sediment, biota, vegetation including food, etc.). This chapter concludes with specific guidance for preparing samples of filters (Section 12.4), wipes (Section 12.5), liquids (Section 12.6), gases (Section 12.7), and bioassay (Section 12.8).

## **12.2 General Guidance for Sample Preparation**

Some general considerations during sample preparation are to minimize sample losses and to prevent contamination. Possible mechanisms for sample loss during preparation steps are discussed in Section 12.2.1, and the contamination of samples from sources in the laboratory is discussed in Section 12.2.2. Control of contamination through cleaning labware is important and described in Section 12.2.3, and laboratory contamination control is discussed in Section 12.2.4.

### **12.2.1 Potential Sample Losses During Preparation**

Materials may be lost from a sample during laboratory preparation. The following sections discuss the potential types of losses and the methods used to control them. The addition of tracers or carriers (Chapter 13) is encouraged at the earliest possible point and prior to any sample preparation step where there might be a loss of analyte. Such preparation steps may include homogenization or sample heating. The addition of tracers or carriers prior to these steps helps to account for any analyte loss during sample preparation.

#### **12.2.1.1 Losses as Dust or Particulates**

When a sample is dry ashed, a fine residue (ash) is often formed. The small particles in the residue are resuspended readily by any flow of air over the sample. Air flows are generated by changes in temperature (e.g., opening the furnace while it is hot) or by passing a stream of gas over the sample during heating to assist in combustion. These losses are minimized by ashing samples at as low a temperature as possible, gradually increasing and decreasing the temperature during the ashing process, using a slow gas-flow rate, and never opening the door of a hot furnace (Section 12.3.1). If single samples are heated in a tube furnace with a flow of gas over the sample, a plug of glass or quartz wool can be used to collect particulates or an absorption

vessel can be used to collect volatile materials. At a minimum, all ash or finely ground samples should be covered before they are moved.

Solid samples are often ground to a fine particle size before they are fused or wet ashed (see Chapters 13 and 14 on dissolution and separation) to increase the surface area and speed up the reaction between the sample and the fluxing agent or acid. Since solid samples are frequently heterogeneous, a source of error arises from the difference in hardness among the sample components. The softer materials are converted to smaller particles more rapidly than the harder ones, and therefore, any loss in the form of dust during the grinding process will alter the composition of the sample. The finely ground particles are also susceptible to resuspension. Samples may be moistened carefully with a small amount of water before adding other reagents. Reagents should be added slowly to prevent losses as spray owing to reactions between the sample and the reagents.

#### 12.2.1.2 Losses Through Volatilization

Some radionuclides are volatile under specific conditions (e.g., heat, grinding, strong oxidizers), and care should be taken to identify samples requiring analysis for these radionuclides. Special preparation procedures should be used to prevent the volatilization of the radionuclide of interest.

The loss of volatile elements during heating is minimized by heating without exceeding the boiling point of the volatile compound. Ashing aids can reduce losses by converting the sample into less volatile compounds. These reduce losses but can contaminate samples. During the wet ashing process, losses of volatile elements can be minimized by using a reflux condenser. If the solution needs to be evaporated, the reflux solution can be collected separately. Volatilization losses can be prevented when reactions are carried out in a sealed tube or a closed metal or Teflon™ bomb. Table 12.1 lists some commonly analyzed radioisotopes, their volatile chemical form, and the boiling point of that species at standard pressure (note that the boiling point may vary based on solution, matrix, etc.).

Often the moisture content, and thus, the chemical composition of a solid is altered during grinding and crushing (Dean, 1995). Decreases in water content are sometimes observed while grinding solids containing essential water in the form of hydrates, likely as a result of localized heating. (See Section 12.3.1.2 for a discussion of the types of moisture present in solid samples.) Moisture loss is also observed when samples containing occluded water are ground and crushed. The process ruptures some of the cavities, and exposes the water to evaporation. More commonly, the grinding process results in an increase in moisture content owing to an increase in

surface area available for absorption of atmospheric water. Both of these conditions will affect the analysis of  $^3\text{H}$  since  $^3\text{H}$  is normally present in environmental samples as  $^3\text{HOH}$ .

**TABLE 12.1 — Examples of Volatile Radionuclides**

Isotope	Chemical Form	Boiling Point (°C)
Tritium — $^3\text{H}$	$\text{H}_2\text{O}$	100
Carbon — $^{14}\text{C}$	$\text{CO}_2$ (produced from $\text{CO}_3^{-2}$ or oxidation of organic material)	-78.5
Iodine — $^{131}\text{I}$ , $^{129}\text{I}$	$\text{I}_2$	185.2 (sublimes readily)
Cesium — $^{134}\text{Cs}$ , $^{135}\text{Cs}$ , $^{137}\text{Cs}$	Cs metal	678.4
	Cs oxides (nitrates decompose to oxides)	~650
	$\text{CsCl}$	1290
Ruthenium — $^{106}\text{Ru}$	$\text{RuO}_4$	40
	$\text{RuCl}_3 \cdot x\text{H}_2\text{O}$	decomposes above 500
Technetium — $^{99}\text{Tc}$	$\text{Tc}_2\text{O}_7$	310.6
	$\text{TcCl}_4$	Sublimes above 300

Source: Greenwood and Earnshaw (1984).

Additional elements that volatilize under specific conditions include arsenic, antimony, tin, polonium, lead, selenium, mercury, germanium, and boron. Osmium is volatilized as the tetroxide under oxidizing conditions similar to those for ruthenium. Carbon, phosphorus, and silicon may be volatilized as hydrides, and chromium is volatilized under oxidizing conditions in the presence of chloride.

### 12.2.1.3 Losses Owing to Reactions Between Sample and Container

Specific elements may be lost from sample materials owing to interaction with a container. Such losses may be significant, especially for trace analyses used in radioanalytical work. Adsorption reactions are discussed in Chapter 10 for glass and plastic containers. Losses owing to adsorption may be minimized by using pretreated glassware with an established hydrated layer. Soaking new glassware overnight in a dilute nitric or hydrochloric acid solution will provide an adequate hydrated layer. Glassware that is used on a regular basis will already have established an adequate hydrated layer. The use of strong acids to maintain a pH less than one also helps minimize losses from adsorption.

Reactions among analytes and other types of containers are described in Table 12.2. Leaving platinum crucibles uncovered during dry ashing to heat samples will minimize reduction of samples to base metals which form alloys with platinum. It is recommended that porcelain not be used for analysis of lead, uranium, and thorium because the oxides of these elements react with porcelain glazes. Increasing the amount of sample for dry ashing increases the amount of ash, allowing trace elements to react with the ash instead of with the container.

TABLE 12.2 — Properties of Sample Container Materials

Material	Recommended Use	Properties
Borosilicate Glass	General applications	Transparent; good thermal properties; fragile; attacked by HF, H <sub>3</sub> PO <sub>4</sub> , and alkaline solutions.
Fused Quartz	High temperature applications	Transparent; excellent thermal properties (up to 1100° C); fragile; more expensive than glass; attacked by HF, H <sub>3</sub> PO <sub>4</sub> , and alkaline solutions.
Porcelain	High temperature applications	Used at temperatures up to 1100° C; less expensive than quartz; difficult to shape; attacked by HF, H <sub>3</sub> PO <sub>4</sub> , and alkaline solutions.
Platinum	High temperature or corrosive applications	Virtually unaffected by acids, including HF; dissolves readily in mixtures of HNO <sub>3</sub> and HCl, Cl <sub>2</sub> water or Br <sub>2</sub> water; adequate resistance to H <sub>3</sub> PO <sub>4</sub> ; very expensive; forms alloys with Hg, Pb, Sn, Au, Cu, Si, Zn, Cd, As, Al, Bi, and Fe, which may be formed under reducing conditions; permeable to H <sub>2</sub> at red heat, which serves as a reducing agent; may react with S, Se, Te, P, As, Sb, B, and C to damage container; soft and easily deformed, often alloyed with Ir, Au, or Rh for strength. Do not use with Na <sub>2</sub> CO <sub>3</sub> for fusion.
Nickel	Molten alkali metal hydroxide and Na <sub>2</sub> O <sub>2</sub> fusions	Suitable for use with strongly alkaline solutions.
Zirconium	Peroxide fusions	Less expensive alternative to platinum; extremely resistant to HCl; resistant to HNO <sub>3</sub> ; resistant to 50% H <sub>2</sub> SO <sub>4</sub> and 60% H <sub>3</sub> PO <sub>4</sub> up to 100° C; resistant to molten NaOH; attacked by molten nitrate and bisulfate; usually available as Zircaloy—98% Zr, 1.5% Sn, trace Fe, Cr, and Ni.
Alumina (Al <sub>2</sub> O <sub>3</sub> )	Acids and alkali melts at low temperatures	Resistant to acids and alkali melts; rapidly attacked by bisulfate melts; brittle, requires thick walled containers.
Polyethylene	Sample and reagent storage	Resistant to many acids; attacked by 16M HNO <sub>3</sub> and glacial acetic acid; begins to soften and lose shape at 60° C; appreciably porous to Br <sub>2</sub> , NH <sub>3</sub> , H <sub>2</sub> S, H <sub>2</sub> O, and HNO <sub>3</sub> (aqueous solutions can lose ~1% volume per year when stored for extended periods of time).
Teflon™	Corrosive applications	Inert to almost all inorganic and organic compounds except F <sub>2</sub> ; porosity to gases is significantly less than that of polyethylene; safe to use at 250° C but decomposes at 300° C; difficulty in shaping containers results in high cost; low thermal conductivity (requires long periods of time to heat samples).

## **12.2.2 Contamination from Sources in the Laboratory**

Contamination leads to biased data that misrepresent the concentration or presence of radionuclides in a specific sample. Therefore, laboratory personnel should take appropriate measures to prevent the contamination of samples. Such precautions are most important when multiple samples are processed together. Possible sources of contamination include:

- Airborne;
- Reagents (tracers are discussed in Chapter 13);
- Glassware/equipment; and
- Facilities.

The laboratory should use techniques that eliminate air particulates or the introduction of any outside material (such as leaks from aerosols) into samples and that safeguard against using contaminated glassware or laboratory equipment. Contamination of samples can be controlled by adhering to established procedures for equipment preparation and decontamination before and after each sample is prepared. Additionally, the results of blank samples (e.g., sand), which are run as part of the internal quality assurance program, should be closely monitored, particularly following the processing of samples with elevated activity.

“Cross-contamination” is the contamination of one sample by another sample that is being processed concurrently or that was processed prior to the current sample leaving a residue on the equipment being used. Simply keeping samples covered whenever practical is one technique to minimize cross-contamination. Another technique is to order the processing of samples beginning with the lowest contamination samples first. It is not always possible to know the exact rank of samples, but historical or field screening data may be useful.

Laboratory personnel should be wary of using the same equipment (gloves, tweezers for filters, contamination control mats, etc.) for multiple samples. Countertops and other preparation areas should be routinely monitored for contamination.

### **12.2.2.1 Airborne Contamination**

Airborne contamination is most likely to occur when grinding or pulverizing solid samples. Very small particles (~10 microns) may be produced, suspended in air, and transported in the air before settling onto a surface. Other sources of potential airborne contamination include samples that already consist of very small particles, or radionuclides that decay through a gaseous intermediate (i.e.,  $^{226}\text{Ra}$  decays to  $^{222}\text{Rn}$  gas and eventually decays to  $^{210}\text{Pb}$ ). Therefore, the

grinding or pulverizing of solid samples or the handling of samples that could produce airborne contamination should be carried out under a laboratory hood to prevent dispersal or deposition in the laboratory of contaminated air particulates. These particles easily can contaminate other samples stored in the area. To prevent such cross-contamination, other samples should be covered or removed from the area while potential sources of airborne contamination are being processed.

If contamination from the ambient progeny of  $^{222}\text{Rn}$  is a concern, this can be avoided by refraining from the use of suction filtration in chemical procedures, prefiltering of room air (Lucas, 1967), and use of radon traps (Lucas, 1963; Sedlet, 1966). The laboratory may have background levels of radon progeny from its construction materials.

#### 12.2.2.2 Contamination of Reagents

Contamination from radiochemical impurities in reagents is especially troublesome in low-level work (Wang et al., 1975). Care must be taken in obtaining reagents with the lowest contamination possible. Owing to the ubiquitous nature of uranium and thorium, they and their progeny are frequently encountered in analytical reagents. For example, Yamamoto et al. (1989) found significant  $^{226}\text{Ra}$  contamination in common barium and calcium reagents. Other problematic reagents include the rare earths (especially cerium salts), cesium salts which may contain  $^{40}\text{K}$  or  $^{87}\text{Rb}$ , and potassium salts. Precipitating agents such as tetraphenyl borates and chloroplatinates may also suffer from contamination problems. In certain chemical procedures, it is necessary to replace inert carriers of the element of interest with non-isotopic carriers when it is difficult to obtain the inert carrier in a contamination-free condition. Devoe (1961) has written an extensive review article on the radiochemical contamination of analytical reagents.

#### 12.2.2.3 Contamination of Glassware/Equipment

Other general considerations in sample preparation include the cleaning of glassware and equipment (Section 12.2.3). Criteria established in the planning documents or laboratory SOPs should give guidance on proper care of glassware and equipment (i.e., scratched glassware increases the likelihood of sample contamination and losses owing to larger surface area). Glassware should be routinely inspected for scratches, cracks, etc., and discarded if damaged. Blanks and screening should be used to monitor for contamination of glassware.

Whenever possible, the use of new or disposable containers or labware is recommended. For example, disposable weigh boats can be used to prevent contamination of a balance. Disposable plastic centrifuge tubes are often less expensive to use than glass tubes that require cleaning after

every use. If non-disposable containers or labware are used, it may be necessary to use new materials for each new project to reduce the potential for contamination. Blanks can be used to detect cross-contamination. Periodic rinsing with a dilute solution of nitric acid can aid in maintaining clean glassware. However, Bernabee et al. (1980) could not easily remove nuclides sorbed onto the walls of plastic containers by washing with strong mineral acids. They report that nuclides can be wiped from the walls, showing the importance of the physical action of a brush to the cleaning process.

#### 12.2.2.4 Contamination of Facilities

In order to avoid contamination of laboratory facilities and possible contamination of samples or personnel, good laboratory practices must be constantly followed and the laboratory must be kept in clean condition. The laboratory should establish and maintain a Laboratory Contamination Control Program (Section 12.2.4) to avoid contamination of facilities and to deal with it expeditiously if it occurs.

### 12.2.3 Cleaning of Labware, Glassware, and Equipment

#### 12.2.3.1 Labware and Glassware

Some labware is too expensive to be used only once (e.g., crucibles, Teflon™ beakers, separatory funnels). Labware that will be used for more than one sample should be subjected to thorough cleaning between uses. A typical cleaning protocol includes a detergent wash, an acid soak (HCl, HNO<sub>3</sub>, or citric acid), and a rinse with deionized or distilled water. As noted in Chapter 10, the use of a brush to physically scrub glassware aids in the removal of contaminants.

The *Chemical Technician's Ready Reference Handbook* (Shugar and Ballinger, 1996) offers practical advice on washing and cleaning laboratory glassware:

- Always clean your apparatus immediately after use. It is much easier to clean the glassware before the residues become dry and hard. If dirty glassware cannot be washed immediately, it should be left in water to soak.
- Thoroughly rinse all soap or other cleaning agent residue after washing glassware to prevent possible contamination. If the surface is clean, the water will wet the surface uniformly; if the glassware is still soiled, the water will stand in droplets.



- Use brushes carefully and be certain that the brush has no exposed sharp metal points that can scratch the glass. Scratched glassware increases the likelihood of sample contamination and losses owing to larger surface areas. Moreover, scratched glassware is more easily broken, especially when heated.

Automatic laboratory dishwashers and ultrasound or ultrasonic cleaners are also used in many radiochemical laboratories. It is important to note that cleaning labware in an automatic laboratory dishwasher alone may not provide adequate decontamination. Contaminated glassware may need to be soaked in acid or detergent to ensure complete decontamination. Ultrasonic cleaning in an immersion tank is an exceptionally thorough process that rapidly and efficiently cleans the external, as well as the internal, surfaces of glassware or equipment. Ultrasonic cleaners generate high-frequency sound waves and work on the principle of “cavitation,” the formation and collapse of submicron bubbles. These bubbles form and collapse about 25,000 times each second with a violent microscopic intensity which produces a scrubbing action (Shugar and Ballinger, 1996). This action effectively treats every surface of the labware because it is immersed in the solution and the sound energy penetrates wherever the solution reaches.

The *Manual for the Certification of Laboratories Analyzing Drinking Water* (EPA, 1992) contains a table of glassware cleaning and drying procedures for the various methods given in the manual (including methods for the analysis of radionuclides in water). The suggested procedure for cleaning glassware for metals analysis is to wash with detergent, rinse with tap water, soak for 4 hours in 20 percent (v/v) HNO<sub>3</sub> or dilute HNO<sub>3</sub> (8 percent)/HCl (17 percent), rinse with reagent water, then air dry. Shugar and Ballinger (1996) suggest treating acid-washed glassware by soaking it in a solution containing 2 percent NaOH and 1 percent disodium ethylenediamine tetraacetate for 2 hours, followed by a number of rinses with distilled water to remove metal contaminants.

More specifically to radionuclides, in their paper discussing the simultaneous determination of alpha-emitting nuclides in soil, Sill et al. (1974) examined the decontamination of certain radionuclides from common labware and glassware:

By far the most serious source of contamination is the cell, electrode, and “O” ring used in the electrodeposition step. Brief rinsing with a strong solution of hydrochloric acid containing hydrofluoric acid and peroxide at room temperature was totally ineffective in producing adequate decontamination. Boiling anode and cell with concentrated nitric acid for 10 to 15 minutes removed virtually all of the activity resulting from the analysis of samples containing less than 500 disintegrations per minute (dpm). When larger quantities of activity such as the  $2.5 \times 10^4$  counts per minute (cpm) used in the material

studies ... had been used, a second boiling with clean acid was generally required. However, boiling nitric acid precipitates polonium and other procedures have to be used in its presence. When such high levels of activity have been used, a blank should be run to ensure that decontamination was adequate before the system is permitted to be used in the analysis of subsequent low-level samples. Prudence suggests that a separate system should be reserved for low-level samples and good management exercised over the level of samples permitted in the low-level system to minimize the number of blanks and full-length counting times required to determine adequate decontamination.

...Beakers, flasks, and centrifuge tubes in which barium sulfate has been precipitated must be cleaned by some agent known to dissolve barium sulfate, such as boiling perchloric or sulfuric acids or boiling alkaline DTPA [diethylenetriaminepentacetate]. This is a particularly important potential source of contamination, particularly if hot solutions containing freshly-precipitated barium sulfate are allowed to cool without stirring. Some barium sulfate post-precipitates after cooling and adheres to the walls so tenaciously that chemical removal is required. Obviously, the barium sulfate will contain whichever actinide is present, and will not dissolve even in solutions containing hydrofluoric acid. Beakers or flasks in which radionuclides have been evaporated to dryness will invariably contain residual activity which generally requires a pyrosulfate fusion to clean completely and reliably. Separatory funnels can generally be cleaned adequately by rinsing them with ethanol and water to remove the organic solvent, and then with hydrochloric-hydrofluoric acids and water to remove traces of hydrolyzed radionuclides...

However, one should note that current laboratory safety guidelines discourage the use of perchloric acid (Schilt, 1979).

#### 12.2.3.2 Equipment

In order to avoid cross-contamination, grinders, sieves, mixers and other equipment should be cleaned before using them for a new sample. Cleaning equipment prior to use is only necessary if the equipment has not been used for some time. The procedure can be as simple or as complicated as the analytical objectives warrant as illustrated by Obenhaus et al. (website reference) in the *SPEX Certiprep Handbook of Sample Preparation and Handling*. In some applications, simply wiping down the equipment with ethanol may suffice. Another practical approach is to brush out the container, and briefly process an expendable portion of the next sample and discard it. For more thorough cleaning, one may process one or more batches of pure quartz sand through the piece of solid processing equipment, and then wash it carefully. The

efficacy of the decontamination is determined by monitoring this sand for radionuclide contamination.

An effective cleaning procedure for most grinding containers is to grind pure quartz sand together with hot water and detergent, then to rinse and dry the container. This approach incorporates a safety advantage in that it controls respirable airborne dusts. It is important to note that grinding containers become more difficult to clean with age because of progressive pitting and scratching of the grinding surface. Hardened steel containers can also rust, and therefore should be dried thoroughly after cleaning and stored in a plastic bag containing a desiccating agent. If rust does occur, the iron oxide coating can be removed by a warm dilute oxalic acid solution or by abrasive cleaning.

#### **12.2.4 Laboratory Contamination Control Program**

The laboratory should establish a general program to prevent the contamination of samples. Included in the program should be ways to detect contamination from any source during the sample preparation steps if contamination of samples occurs. The laboratory contamination control program should also provide the means to correct procedures to eliminate or reduce any source of contamination. Some general aspects of a control program include:

- Appropriate engineering controls, such as ventilation, shielding, etc., should be in place.
- The laboratory should be kept clean and good laboratory practices should be followed. Personnel should be well-trained in the safe handling of radioactive materials.
- Counter tops and equipment should be cleaned and decontaminated following spills of liquids or dispersal of finely powdered solids. Plastic-backed absorbent benchtop coverings or trays help to contain spills.
- There should be an active health physics program that includes frequent monitoring of facilities and personnel.
- Wastes should be stored properly and not allowed to accumulate in the laboratory working area. Satellite accumulation areas should be monitored.
- Personnel should be mindful of the use of proper personnel protection equipment and practices (e.g., habitual use of lab coats, frequent glove changes, routine hand washes).

- Operations should be segregated according to activity level. Separate equipment and facilities should be used for elevated and low-level samples whenever possible.

- SOPs describing decontamination and monitoring of labware, glassware, and equipment should be available.

- Concentrated standard stock solutions should be kept isolated from the general laboratory working areas.

As an example, Kralian et al. (1990) have published the guidelines for effective low-level contamination control.

### **12.3 Solid Samples**

This section discusses laboratory preparation procedures for solid samples as illustrated in Figure 12.2. General procedures such as exclusion of unwanted material in the sample; drying, charring, and ashing of samples; obtaining a constant weight (if required); and homogenization are discussed first. Examples of preparative procedures for solid samples are then presented.

Solid samples may consist of a wide variety of materials, including:

- Soil and sediment;
- Biota (plants and animals); and
- Other materials (metal, concrete, asphalt, solid waste, etc.).

Before a solid sample is prepared, the specific procedures given in the planning documents should be reviewed. This review should result in a decision that indicates whether materials other than those in the intended matrix should be removed, discarded, or analyzed separately. Any material removed from the sample should be identified, weighed, and documented.

To ensure that a representative aliquant of a sample is analyzed, the sample should first be dried or ashed and then blended or ground thoroughly (Appendix F). Homogenization should result in a uniform distribution of analytes and particles throughout the sample. The size of the particles that make up the sample will have a bearing on the representativeness of each aliquant.

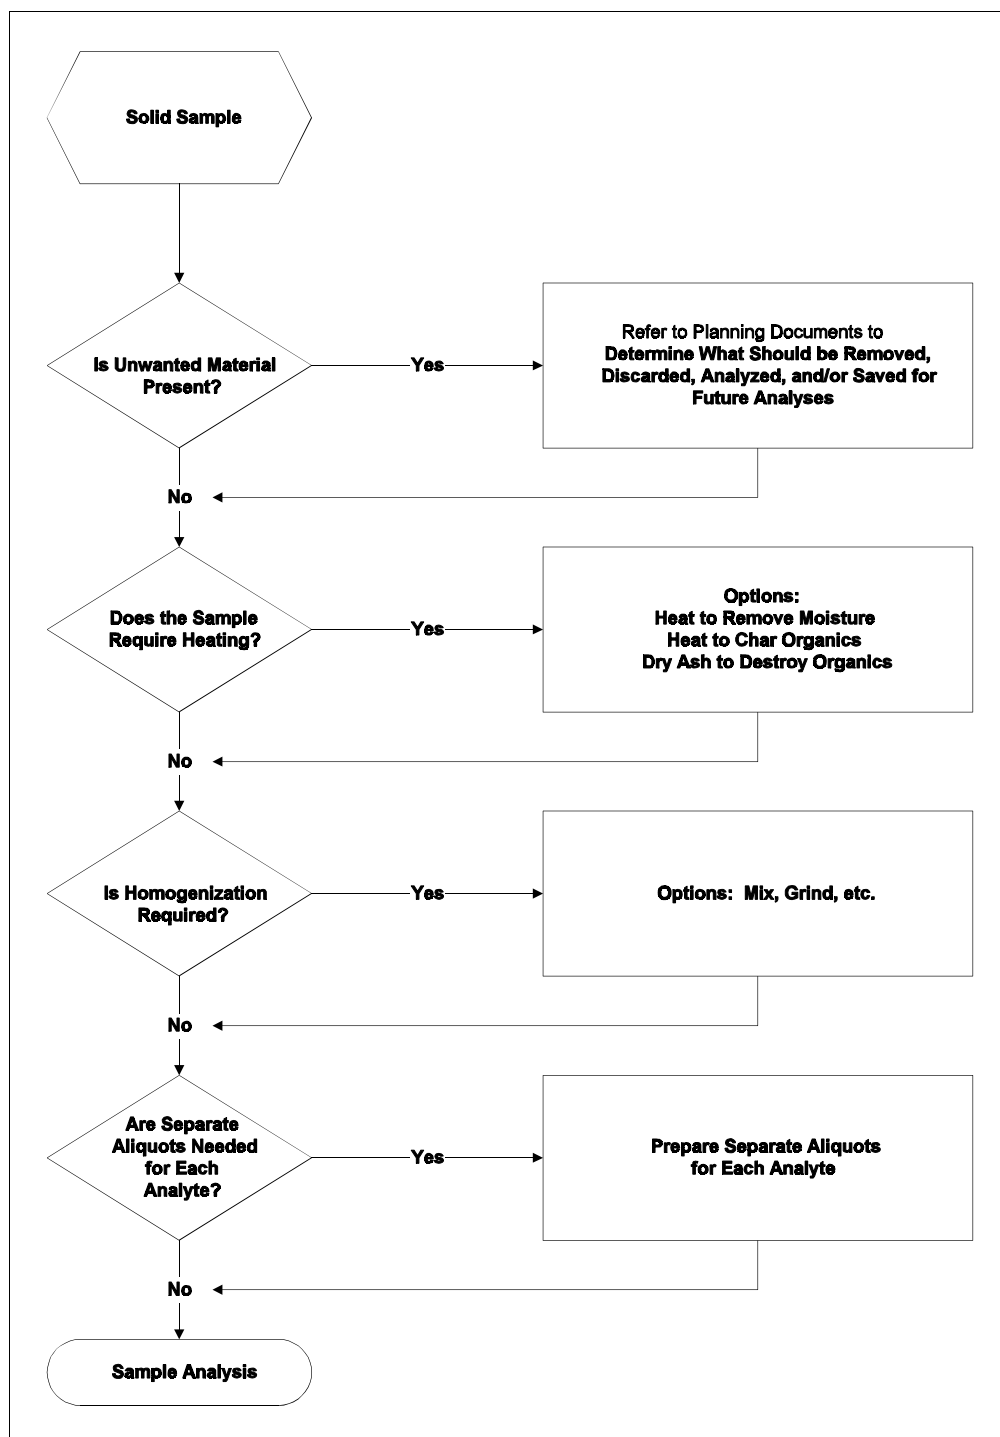


FIGURE 12.2—Laboratory Sample Preparation Flowchart (for Solid Samples)

### 12.3.1 General Procedures

The following sections discuss the general procedures for exclusion of material, heating solid samples (drying, charring, and ashing), obtaining a constant weight, mechanical manipulation (grinding, sieving, and mixing), and subsampling. Not every step is done for all solid sample categories (soil/sediment, biota, and other) but are presented here to illustrate the steps that could be taken during preparation.

#### 12.3.1.1 Exclusion of Material

*Exclusion of Material by Size and Particles.* During solid preparation, some particles may be identified in the sample that are not a part of the matrix intended for analysis. Examples of such particles are rocks and pebbles or fragments of glass and plastic. Depending on the specific procedures given in the planning documents on the constitution of the sample taken, rocks and pebbles can be removed and analyzed separately if desired. The sample should be weighed before and after any material is removed. Other materials that are not a part of the required matrix can also be removed and analyzed separately. If analysis of the material removed is necessary, applicable SOPs should be used to prepare the material for analysis.

*Exclusion of Organic Material.* Leaves, twigs, and grass can easily be collected inadvertently along with samples of soil or sediment. Because these are not usually intended for analysis, they are often removed and stored for future analysis, if necessary. The material removed should be identified, if possible, and weighed.

#### 12.3.1.2 Principles of Drying Techniques

Applying elevated temperatures during sample preparation is a widely used technique for the following reasons:

- To remove moisture or evaporate liquids (raise the temperatures to 60° to 110° C).
- To prepare organic material for subsequent wet ashing or fusion (“char” the material by heating to medium temperature of 200° to 300° C).
- To prepare the sample for subsequent determination of nonvolatile constituents (dry ash at high temperature of 450° to 750° C).

Once a decision is made to use elevated temperatures during sample preparation, several questions should be considered:

- What material should be used for the sample container?
- What should serve as the heat source?
- How quickly should the temperature be raised? (Rate of stepwise temperature increase)
- What is the maximum temperature to which the sample should be exposed?
- How long should the sample be heated at the maximum temperature?
- How quickly should the sample be cooled afterward?

The following sections provide information related to these questions.

Note that there are times during sample preparation when samples should not be heated. For example, samples to be prepared for  $^3\text{H}$  or  $^{14}\text{C}$  determination should not be heated. Since  $^3\text{H}$  is normally present as tritiated water in environmental samples, heating will remove the  $^3\text{H}$ . Similarly,  $^{14}\text{C}$  is usually present in environmental samples as carbonates or  $^{14}\text{CO}_2$  dissolved in water, and heating will release  $^{14}\text{C}$  as a gas. Samples to be analyzed for iodine, mercury, antimony, or other volatile elements should be heated only under conditions specified in the planning documents. If both volatile and nonvolatile elements are determined from the same sample, aliquants of the original sample should be removed for determination of the volatile elements.

Ovens, furnaces, heat lamps, and hot plates are the traditional means to achieve elevated temperatures in the laboratory. However, more recently, microwave ovens have added an additional tool for elevating temperature during sample preparation. Walter et al. (1997) and Kingston and Jassie (1988) give an overview of the diverse field of microwave-assisted sample preparation. A dynamic database of research articles related to this topic can be found at the SamplePrep Web™ at <http://www.sampleprep.duq.edu/index.html>. As microwave sample preparation has developed, numerous standard methods with microwave assistance have been approved by the American Society for Testing and Materials (ASTM), Association of Official Analytical Chemists (AOAC), and the U.S. Environmental Protection Agency (EPA). The majority of the microwave-assisted methods are for acid-dissolution (Chapter 13), but several are for drying samples.

Alternatives to heating samples include drying them slowly in a vacuum desiccator, air-drying, or freeze-drying. ASTM D3974 describes three methods of preparing soils, bottom sediments, suspended sediments, and waterborne materials: (1) freeze-drying; (2) air-drying at room temperature; and (3) accelerated air-drying.

### *Drying Samples*

It must be determined at the start of an analytical procedure if the results are to be reported on an *as-received* or *dry-weight* basis. Most analytical results for solid samples should be reported on a dry-weight basis, which denotes material dried at a specified temperature to a constant weight or corrected through a “moisture” determination made on an aliquant of the sample taken at the same time as the aliquant taken for sample analysis.

Typically, samples are dried at temperatures of 105° to 110° C. Sometimes it is difficult to obtain constant weight at these temperatures, then higher temperatures must carefully be used. Alternatively, for samples that are extremely heat sensitive and decompose readily, vacuum desiccation or freeze-drying techniques are applicable.

The presence of water in a sample is a common problem frequently facing the analyst. Water may be present as a contaminant (i.e., from the atmosphere or from the solution in which the substance was formed) or be bonded as a chemical compound (i.e., a hydrate). Regardless of its origin, water plays a role in the composition of the sample. Unfortunately, especially in the case of solids, water content is variable and depends upon such things as humidity, temperature, and the state of subdivision. Therefore, the make-up of a sample may change significantly with the environment and the method of handling.

Traditionally, chemists distinguish several ways in which water is held by a solid (Dean, 1995).

- Essential water is an integral part of the molecular or crystal structure and is present in stoichiometric quantities, for example,  $\text{CaC}_2\text{O}_4 \cdot 2\text{H}_2\text{O}$ .
- Water of constitution is not present as such in the solid, but is formed as a product when the solid undergoes decomposition, usually as a result of heating. For example,  $\text{Ca}(\text{OH})_2 \rightarrow \text{CaO} + \text{H}_2\text{O}$ .
- Nonessential water is retained by physical forces, is non-stoichiometric, and is not necessary for the characterization of the chemical composition of the sample.



- Absorbed water is retained on the surface of solids in contact with a moist environment, and therefore, is dependent upon the humidity, temperature, and surface area of the solid.
- Sorbed water is encountered with many colloidal substances such as starch, charcoal, zeolite minerals, and silica gel and may amount to as much as 20 percent or more of the solid. Sorbed water is held as a condensed phase in the interstices or capillaries of the colloid and it is greatly dependent upon temperature and humidity.
- Occluded water is entrapped in microscopic pockets spaced irregularly throughout solid crystals. These cavities frequently occur naturally in minerals and rocks.
- Water also may be present as a solid solution in which the water molecules are distributed homogeneously throughout the solid. For example, natural glasses may contain several percent moisture in this form.

*Heat Source.* There are several choices when heating to dryness. The heat source is often determined by the amount of time available for drying and the potential for the sample to spatter or splash during drying. When time is not a primary concern and there is little or no chance of sample cross-contamination, samples are heated uncovered in a drying oven at the minimum temperature needed to remove moisture. If time is of concern, samples with high moisture content can usually be dried or evaporated faster using a hot plate. Heating on a hot plate significantly increases the chance of cross-contamination by spattering or splashing during boiling. However, ribbed watch glasses, which cover the sample yet still allow for evaporation, can be used to minimize cross contamination in this approach. Samples may also be placed under a heat lamp. This method reduces the risk of cross-contamination by applying heat to the surface where vaporization occurs, minimizing splashing during boiling. However, the elevated temperature is difficult to measure or control, and spattering still may be a problem when the sample reaches dryness.

Microwave systems may also be used to dry samples. ASTM E1358 and ASTM D4643 use microwave energy to dry either wood or soil to a constant weight. In a similar fashion, AOAC Methods 985.14 and 985.26 use microwave energy to dry fat from meat or water from tomato juice. Other examples include Beary (1988) who has compared microwave drying to conventional techniques using NIST solid standards (coal, clays, limestone, sediment) and foods and food materials (rice and wheat flour) standards and Koh (1980) who discusses microwave drying of biological materials.

*Container Material.* A sample container's material composition typically poses no problem. Borosilicate glass is generally recommended because it is inexpensive, transparent, reusable, and has good thermal properties. Platinum, Teflon™ (polytetrafluoroethylene—PTFE), porcelain, or aluminum foil containers are acceptable and may be preferable in certain situations. Polyethylene and other plastics of low melting point are only useful in hot water baths or ovens where the temperature is closely monitored. If polyethylene is going to be used, be aware that it is affected by heat applied directly to the container. The properties of several common materials used for sample containers are presented in Table 12.2 (on page 12-5). Note that the sample containers commonly received from the field will be those suitable for bulk samples rather than containers used during sample preparation. The plan will identify the type of container material to be used for field activities for samples to be shipped to the laboratory and the type of container material to be used during the various steps of sample preparation.

*Heating Rate.* The heating rate is generally not considered when removing moisture, because the maximum temperature typically is very low (60° to 110° C). Samples simply are placed inside the preset oven. Hot plates may be preheated to the desired temperature before heating the sample or turned on and gradually heated with the sample in place.

*Maximum Temperature.* The maximum temperature used for drying samples typically is just above the boiling point of water—105° to 110° C. Higher temperatures will not dry the samples significantly faster and may result in accidents or cross-contamination due to uneven heating. Lower temperatures will not reduce the chance of cross-contamination, but will significantly increase the drying time. One exception to this rule occurs when the physical form of the sample needs to be preserved. Many minerals and chemicals have waters of hydration that affect the structure and may also affect the chemical and physical properties. Samples heated at 60° C will retain the waters of hydration in most chemicals and minerals and still provide dry samples in a reasonable period of time (e.g., 12 to 15 hrs.).

*Time.* The duration a sample is heated to remove moisture depends on the size of the sample, the amount of moisture in the sample, the air flow around the sample, and the temperature applied to the sample. If heating the sample is to provide a constant dry weight, it is more difficult to determine how long to heat the sample. One convenient approach, especially when working with numerous samples, is to dry all materials overnight, or occasionally longer. This amount of heating is usually more than sufficient for drying samples for radiochemical analysis. If time is a critical factor or if a quantitative assessment of the uncertainty in the sample weight is required by the planning documents, the sample can be subjected to repeated cycles of drying and weighing until a series of weights meet the specified requirements (Section 12.3.1.3). For example, one such requirement might be to obtain three consecutive weights with a standard

deviation less than 5 percent of the mean. While repeated cycles of drying and weighing can provide a quantitative measure of the uncertainty in the sample weight over time, a single weight after an overnight drying cycle typically provides a similar qualitative level of confidence with significantly less working time. Another time-saving step is to use microwave techniques rather than conventional heating sources during sample preparation (ANL/ACL, 1992; Walter et al., 1997).

*Alternatives to Heating.* (1) Vacuum-desiccation. A desiccator is a glass or aluminum container that is filled with a substance that absorbs water, a “desiccant.” The desiccator provides a dry atmosphere for objects and substances. Dried materials are stored in desiccators while cooling in order to minimize the uptake of ambient moisture. The ground-glass or metal rim of the desiccator should be greased lightly with petroleum jelly or silicone grease to improve performance. Calcium sulfate, sodium hydroxide, potassium hydroxide, and silica gel are a few of the common desiccants. The desiccant must be renewed frequently to keep it effective. Surface caking is a signal to renew or replace the desiccant. Some desiccants contain a dye that changes color upon exhaustion.

Vacuum desiccators are equipped with a side-arm so that they may be connected to a vacuum to aid in drying. The contents of the sealed evacuated desiccator are maintained in a dry, reduced-pressure atmosphere. Care must be exercised when applying a vacuum as a rapid pressure reduction, for high water content samples can result in “boiling” with subsequent sample loss and potential cross-contamination.

(2) Freeze-drying. Certain substances (i.e., biological materials, pharmaceuticals), which are extremely heat sensitive and cannot be dried at atmospheric conditions, can be freeze-dried (Cameron and Murgatroyd, 1996). Freeze-drying, also known as “lyophilization,” is the process by which substances are frozen, then subjected to high vacuum. Under these conditions ice (water) sublimates and other volatile liquids are removed. The non-sublimable material is left behind in a dry state.

To freeze-dry effectively, dilute solutions are used. In order to increase the surface area, the material is spread out on the inner surface of the container as it is frozen. Once the solution or substance to be dried is frozen solid, the primary drying stage begins in which a high vacuum is applied, and the ice sublimates, desorbing the free ice and some of the bound moisture. During secondary drying, a prolonged drying stage, the sorbed water which was bound strongly to the solids, is converted to vapor. This can be a slow process because the remaining bound water has a lower pressure than the free liquid at the same temperature, making it more difficult to remove.

Secondary drying actually begins during the primary drying phase, but it must be extended after the total removal of free ice to achieve low levels of residual moisture.

Commercial freeze-drying units are self contained. Simple units consist of a vacuum pump, adequate vapor traps, and a receptacle for the material to be dried. More sophisticated models include refrigeration units to chill the solutions, instrumentation to designate temperature and pressure, heat and cold controls, as well as vacuum-release valves. The vacuum pump should be protected from water with a dry-ice trap and from corrosive gases with chemical gas-washing towers.

#### *Charring of Samples to Partially Oxidize Organic Material*

Heating samples at a moderate temperature (200° to 300° C) is sometimes used as a method of preparing a sample for subsequent decomposition using wet ashing or fusion techniques. Large amounts of organic material can react violently or even explosively during decomposition. Heating the sample to partially oxidize—or “char”—the organic material may limit reactivity during subsequent preparation.

*Heat Source.* Heat lamps, muffle furnaces, or hot plates may be used as a heat source for charring samples. Heat lamps are often selected because they can also be used to dry the sample before charring. Once dried, the sample can be moved closer to the lamp to raise the temperature and char the sample (confirmed by visual inspection). Heat lamps also reduce the potential for cross-contamination by minimizing spattering and splashing. Hot plates can be used similarly to heat lamps. The sample is dried and the temperature is raised to char the sample; however, hot plates increase the probability of spattering and splashing. Muffle furnaces can be used when the charring is performed as part of dry ashing instead of part of the drying process. In this case, the muffle furnace temperature is first raised slowly.

*Sample Container.* The choice of sample container depends primarily on the next step in the sample preparation process. When dry ashing or fusing, the sample container will usually be a platinum or porcelain crucible. Zirconium or nickel crucibles may also be used. If the sample will be dissolved using wet ashing techniques, the container may be borosilicate glass or a platinum crucible. Care should be taken to prevent ignition of samples in glass containers. Ignited samples may burn at temperatures high enough to cause damage to the container and loss of sample. Polyethylene and Teflon™ generally are not acceptable because of the increased temperature and risk of melting the container.

*Heating Rate.* Heating rate becomes a concern when charring samples because of the increased temperatures. The general rule is to raise the temperature slowly to heat the sample evenly and prevent large increases in temperature within the sample, which could lead to ignition. Typically, a rate of 50° to 100° C per hour is considered appropriate. Samples containing large quantities of organic material may require slower heating rates.

*Maximum Temperature.* One of the primary goals of charring a sample is to oxidize the materials slowly and gently. Gentle oxidation is accomplished by slowly raising the temperature close to the ignition point and letting the sample smolder. Many organic compounds ignite in the range of 200° to 300° C (e.g., paper burns at 230° C), so this is usually the range of temperatures where charring takes place. Ignition results in rapid oxidation accompanied by large volumes of released gases and potential sample loss. This reaction can raise the temperature of the sample to several hundred degrees above the desired maximum and result in significant losses during off-gassing. The progress of the reaction can be monitored visually by observing the volume of gas or smoke released. Thin wisps of smoke are usually allowable; clouds of smoke and flames are not. Visual inspection is easily accomplished when hot plates or heat lamps are used as heat sources. Some muffle furnaces are fitted with viewing windows to allow visual inspection. Never open a muffle furnace just to check on the progress of a reaction. This will cause a sudden change in temperature, increase the oxygen level and possibly ignite the sample, and disrupt air currents within the furnace to increase potential sample loss.

*Time.* The duration required to char a sample depends on the sample size, the amount of organic material in the sample, the ignition point of the organic material, the temperature of the sample, and the oxygen supply. Samples usually are heated until smoke begins to appear and allowed to remain at that temperature until no more smoke is evident. This process is repeated until the temperature is increased and no more smoke appears. Charring samples may require a significant amount of time and effort to complete. The duration may be reduced by improving the flow of air to the sample or mixing HNO<sub>3</sub> or nitrate salts with the sample before drying. However, this approach is recommended only for well-characterized samples, those previously evaluated for the applicability of this technique, because nitrated organic compounds can oxidize in a violent or explosive manner.

#### *Dry Ashing Samples*

The object of dry ashing is to combust all of the organic material and to prepare the sample for subsequent treatment using wet ashing or fusion techniques. This procedure involves heating a sample in an open dish or crucible in air, usually in a muffle furnace to control the temperature and flow of air. Microwave techniques are also available for dry ashing samples.

Dry ashing is used to determine ash weight as well as nonvolatile constituents. The associated chemistry is very complex, with oxidizing and reducing conditions varying throughout the sample and over time. During the combustion process, temperatures in the sample may reach several hundred degrees above the desired temperature, particularly if there is good air flow at the beginning of the ashing process (Bock, 1979). Covering samples during heating is not recommended, especially when using platinum crucibles. The lack of air produces a reducing atmosphere that results in reduction of metals that alloy with the crucible (Table 12.2 on page 12-5). This reaction results in loss of sample and potential for contamination of subsequent samples when using the same crucible.

*Heat Source.* The traditional heat sources for dry ashing are muffle furnaces or burner flames. Electronic muffle furnaces are recommended for all heating of platinum crucibles because burners produce significant levels of hydrogen gas during combustion, and platinum is permeable to hydrogen gas at elevated temperatures. Hydrogen gas acts as a reducing agent that can result in trace metals becoming alloyed to the platinum.

Microwave ovens have also proved to be quick and efficient when dry ashing plant tissue samples, with results comparable to conventional resistance muffle furnaces (Zhang and Dotson, 1998). The microwave units are fitted with ashing blocks (a ceramic insert) which absorb microwave energy and quickly heats to high temperatures. This, in combination with the microwave energy absorbed directly by the sample, allows for rapid dry ashing of most materials. The units are designed for increased air flow which further accelerates combustion of the samples.

*Sample Container.* Platinum, zirconium, or porcelain are usually used to form crucibles for dry ashing. Nickel may also be appropriate for some applications (Table 12.2). Platinum generally is recommended when available and is essentially inert and virtually unaffected by most acids. Zirconium and porcelain crucibles are resistant to most acids, are more resistant to HCl, and are significantly less expensive than platinum. Glass and plastic containers should not be used for dry ashing because the elevated temperatures exceed the melting point of these materials.

Crucibles fabricated from ceramic, graphite, and platinum can be used in microwave applications. Quartz fiber crucibles can accelerate the ashing process since this material rapidly cools and allows many sample types to be reweighed in 60 seconds or less after removal from the microwave unit.

*Heating Rate.* Samples should be dried before dry ashing and placed in an unheated furnace; then, the furnace temperature is gradually increased. The sample should be spread as thinly and

evenly as possible on the bottom of the container to allow for its equal heating. To ensure even heating of the sample and to minimize the chance of ignition, the temperature of the furnace is raised slowly. If the sample was previously charred, a rate of approximately 100° C per hour is typical. This rate is slow enough that small amounts of organic material or water can be removed from the sample without violent reactions. If the sample is not charred and contains a significant amount of organic material, a slower rate may be necessary to control the oxidation of organic material.

**Maximum Temperature.** The maximum temperature is determined by the sample matrix and the volatility of the elements to be analyzed. Generally, the temperature should be as low as possible to reduce the loss of volatile compounds, but high enough to ensure complete combustion of the sample. A minimum temperature of 450° C is often used to ensure complete combustion (Bock, 1979). The upper limit for dry ashing is usually determined by the sample container and the elements being analyzed and is generally considered to be 750° C, but sample-specific conditions may use temperatures up to 1,100° C. However, in practice, some components which are normally considered to be nonvolatile may be lost at temperatures above 650° C (Bock, 1979). Ashing aids may be added to samples to accelerate oxidation, prevent volatilization of specific elements, and prevent reaction between the sample and the container. Examples include adding nitrate before drying to assist oxidation and loosen the ash during combustion, adding sulfate to prevent volatilization of chlorides (e.g., PbCl<sub>2</sub>, CdCl<sub>2</sub>, NaCl) by converting them to the higher boiling sulfates, and adding alkaline earth hydroxides or carbonates to prevent losses of anions (e.g., Cl<sup>-</sup>, As<sup>-3</sup>, P<sup>-3</sup>, B). Table 12.3 lists dry ashing procedures using a platinum container material for several elements commonly determined by radiochemical techniques.

**TABLE 12.3 — Examples of Dry-Ashing Temperatures (Platinum Container)**

Element	Temperature/Matrix
Cobalt	450° to 600° C for biological material; some losses reported owing to reactions with crucible; increased volume of sample increases volume of ash and limits loss of sample.
Cesium	400° to 450° C for food and biological material; CsCl and CsNO <sub>3</sub> volatilize at temperatures above 500° C.
Iodine	400° to 500° C with an alkaline ashing aid to prevent volatilization; losses reported as low as 450° C; total volatilization >600° C.
Lead	450° to 500° C acceptable for most samples; bone or coal (lead phosphate) may be ashed as high as 900° C without significant losses; PbO <sub>2</sub> reacts with silica in porcelain glaze at low temperatures; PbCl <sub>2</sub> is relatively volatile and nitrate or sulfate ashing aids have been used to good effect.
Plutonium	450° C with nitric acid ashing aid for biological material, 550° C for dust on air filters, 700° C for soil; high temperature leads to adsorption onto carbon particles and incomplete dissolution of ash.
Strontium	450° to 550° C for plants, 600° C for meat, 700° C for milk and bone.

## Laboratory Sample Preparation

Element	Temperature/Matrix
Technetium	725° to 750° C for plants treated with ammonia.
Thorium	750° C.
Uranium	600° C for coal, 750° C for biological material; uranium reacts with porcelain glaze resulting in sample losses.

Source: Bock (1979).

(Note that reducing conditions for platinum containers are given in Table 12.2)

*Time.* The duration required to completely combust a sample depends on the size of the sample, the chemical and physical form of the sample before and after ashing, and the maximum temperature required to ash the sample. In many cases, it is convenient to place the sample in an unheated furnace and gradually raise the temperature during the day until the maximum temperature is achieved. The furnace is then left at the maximum temperature overnight (12 hours). The furnace is allowed to cool during the next day, and samples are removed from a cold oven. This procedure helps prevent sudden changes in temperature that could cause air currents which may potentially disturb the ash. An alternative is to leave the sample at maximum temperature for 24 hours and let the sample cool in the oven the second night to ensure complete combustion of the sample.

The elapsed time for dry ashing samples can be significant (greater than 36 hours), but the actual time required by laboratory personnel is minimal.

### 12.3.1.3 Obtaining a Constant Weight

If required, constant weight is obtained by subjecting a sample to repetitive cycles of drying and weighing until a series of weights meets specified requirements. Project-specific planning documents or laboratory SOPs should define the acceptance criteria. For example, in the methods for Total Dissolved Solids and Total Suspended Solids, from the *Standard Methods for the Examination of Water and Wastewater* (Greenberg et al., 1992), solids are repetitively heated for an hour, then weighed until successive weighings agree within 4 percent of the mass or within 0.5 mg. In the ASTM guidelines for the preparation of biological samples (ASTM D4638), an accurately weighed sample (1 to 2 g  $\pm$  0.1 mg, 5 to 10 g  $\pm$  1 mg, >10 g  $\pm$  10 mg) is heated for 2 hours, cooled in a desiccator, and weighed. Drying is repeated at hourly intervals to attain a constant weight within the same accuracy.

Laboratory conditions, calibration of the balance, dynamic range of the balance, drying techniques, drying vessel material, sample transfer techniques, weighing technique, taring and re-taring the balance, recording techniques, data manipulation and modeling all impact the



uncertainty of determining the mass of the sample. At the National Institute of Science and Technology (NIST), samples are dried to constant weight when taking a sample for analysis, calibrating carriers, and recovering carriers after radiochemical separations. To minimize the weighing uncertainty:

- Balances are calibrated annually with weights traceable to NIST.
- The balance is on a vibration resistant table in a low air turbulence area and, when possible, the weighing room is on grade level.
- Clean plastic, glass, or metal weighing containers are used at temperatures well below their softening point.
- Samples are ground to provide consistent particle size and surface area for reproducible drying.
- Temperature or vacuum ramp and duration are designed to provide stoichiometric consistency and cooled in desiccators.
- Once desiccators are opened, masses are corrected for absorption of moisture from the air.
- Weighings are conducted in a temperature and humidity controlled room.
- The calibrated 5 decimal place balance is double shielded from drafts with a lucite enclosure box.
- The operator sits in front of the balance for about 10 minutes before weighing begins to warm the balance with body heat.
- Temperature, pressure and relative humidity are recorded periodically to correct for air buoyancy.
- Disposable gloves are used to prevent transfer of finger oils to the sample container.
- “Zero” or tares are periodically taken to monitor fluctuations and drift in the balance operation.
- The operator tries to sight the readings off the scale reproducibly.

- After a weight has been put on or taken off of the pan, the balance is allowed to settle for about 1 minute before a reading is taken.
- When possible, an electronic balance is used for recording the masses through a cable linked to a computer. In the absence of an electronic balance, two operators are used to read and record the masses.
- Moisture absorption models are assessed for realistic extrapolation to the time when the sample was taken from the desiccator, and uncertainties are assigned at  $t = 0$  and for differences among models.
- All decimal places are carried until the final value is reported.
- Replicate drying of several samples are used to validate the efficacy of the drying protocol before routine use.

Among this list, major contributors to uncertainty are reaching stoichiometric consistency in the dried sample, calibration of the balance, fluctuation and drift in the balance operation, and curve-fitting moisture absorption corrections. These sources of measurement uncertainties should be quantified by measurement, inference, or judgement, then combined in quadrature as the mass uncertainty.

#### 12.3.1.4 Subsampling

Laboratories routinely receive larger samples than required for analysis. The challenge then becomes to prepare a sample that is representative and large enough for analysis, but not so large as to cause needless work in its final preparation. Generally, a raw sample first is crushed to a reasonable particle size and a portion of the crushed material is taken for analysis. This step may be repeated with intermittent sieving of the material until an appropriate sample size is obtained. Then, this final portion is crushed to a size that minimizes sampling error and is fine enough for the dissolution method (Dean 1995; Pitard, 1993).

French geologist Pierre Gy (1992) has developed a theory of particulate sampling, which is applicable to subsampling in the laboratory. Appendix F summarizes important aspects of the theory and includes applications to radiochemistry. Some of the important points to remember include the following:

- For most practical purposes, a subsample is guaranteed to be unbiased only if every particle in the sample has the same probability of being selected for the subsample.
- The weight of the subsample should be many times greater than the weight of the largest particle in the sample.
- The variance associated with subsampling may be reduced either by increasing the size of the subsample or by reducing the particle sizes before subsampling.
- Grouping and segregation of particles tends to increase the subsampling variance.
- Grouping and segregation can be reduced by increment sampling, splitting, or mixing.

*Increment sampling* is a technique in which the subsample is formed from a number of smaller portions selected from the sample. A subsample formed from many small increments will generally be more representative than a subsample formed from only one increment. The more increments the better. An example of increment sampling is the one-dimensional “Japanese slab-cake” method (Appendix F).

*Splitting* is a technique in which the sample is divided into a large number of equal-sized portions and several portions are then recombined to form the subsample. Splitting may be performed by a manual procedure, such as fractional shoveling (Appendix F), or by a mechanical device, such as a riffle splitter. A riffle splitter consists of a series of chutes directed alternately to opposite sides. The alternating chutes divide the sample into many portions, which are then recombined into two. The riffle may be used repeatedly until the desired sample size is obtained. Riffle splitters are normally used with free-flowing materials such as screened soils.

Another traditional method for splitting is coning and quartering (Appendix F). Gy (1992) and Pitard (1993) do not recommend coning and quartering because with similar tools and effort, one can do fractional shoveling, which is a more reliable method.

If proper techniques and tools are used and adequate care is taken, samples of the sizes typically encountered in the laboratory can be mixed effectively. However, the effects of mixing tend to be short-lived because of the constant influence of gravity. Heterogeneous material may begin to segregate immediately after mixing.

The method and duration needed to mix a sample adequately depends on the volume and type of material to be mixed. Small volumes can be mixed by shaking for a relatively short time. Large

volumes may require hours. Pitard (1993) describes dynamic and discontinuous processes for mixing samples including:

- Mechanical mixing of test tube samples is useful for small sample size and can be performed on many samples at once. Some examples are a pipette shaker with a motor-activated, rocking controlled motion; a nutator mixer with the test tubes fixed to an oscillating plate; and a tube rotator where tubes are attached to a rotating plate mounted at an angle.
- Mechanical mixing of closed containers by rotating about a tumbling axis. A turbula mechanical mixer is an example.
- Magnetic stirrers are commonly used to homogenize the contents of an open beaker.
- V-blenders are used to homogenize samples from several hundred grams to kilogram size.
- Stirrers coupled with propellers or paddles are used to mix large volumes of slurries or pulp.
- Sheet mixing or rolling technique, in which the sample is placed on a sheet of paper, cloth, or other material, and the opposite corners are held while rolling the sample (see ASTM C702 for aggregates).
- Ball and rod mills homogenize as well as grind the sample (see ASTM C999 for soils).

When dealing with solid samples, it is often necessary to grind the sample to reduce the particle size in order to ensure homogeneity and to facilitate attack by reagents. The *SPEX CertiPrep Handbook of Sample Preparation and Handling* (Obenauf et al., website reference) is an excellent resource for information regarding grinding and blending.

For hand grinding, boron carbide mortars and pestles are recommended. For samples which can be pulverized by impact at room temperature, a shatterbox, a mixer-mill, or a Wig-L-Bug™ is appropriate, depending on the sample size. For brittle materials—such as wool, paper, dried plants, wood, and soft rocks—which require shearing as well as impact, a hammer-cutter mill is warranted. For flexible or heat-sensitive samples such as polymers, cereal grains, and biological materials, cryogenic grinding is necessary. Methods are described below:

- A shatterbox spins the sample, a puck, and a ring inside a dish-shaped grinding container in a tight, high-speed horizontal circle. Within two to five minutes, approximately 100 grams of brittle material can be reduced to less than 200 mesh. Shatterboxes are typically used to grind

soils, cement mix, rocks, slags, ceramics, and ores. They have also been used for hundreds of other materials including dried marsh-grass, pharmaceuticals, fertilizers, and pesticides. When used in a cryogenic atmosphere, this approach can be used to grind rubber, polymers, bone, hair, and tissue.

- A mixer-mill grinds samples by placing them in a container along with one or more grinding elements and imparting motion to the container. The containers are usually cylindrical, and the grinding elements are ordinarily balls, but may be rods, cylinders or other shapes. As the container is rolled, swung, vibrated or shaken, the inertia of the grinding elements causes them to move independently into each other and against the container wall, thus, grinding the sample. Mixer-mills are available for a wide-range of sample sizes. The length of time necessary to grind a sample depends on the hardness of the material and the fineness desired in the final product.
- The Wig-L-Bug™ is an effective laboratory mill for pulverizing and blending very small samples, typically in the range of 0.1 to 1 mL.
- A hammer-cutter mill utilizes high-speed revolving hammers and a serrated grinding chamber lining to combine both shearing and impact. A slide at the bottom of the hopper feeds small portions of the sample (up to 100 mL) into the grinding chamber. After the sample is adequately pulverized, it passes through a perforated-steel screen at the bottom of the grinding chamber and is then collected. With this approach, dried plants and roots, soils, coal and peat, chemicals, and soft rocks all grind quickly with little sample loss.
- Many analytical samples—such as polymers, rubber, and tissues that are too flexible or susceptible to degradation to be impact-ground at room temperature—can be embrittled by chilling, and then pulverized. Samples can be frozen and placed in a traditional grinder, or alternatively, a freezer mill can be utilized. In a freezer mill, the grinding vial is immersed in liquid nitrogen and an alternating magnetic field shuttles a steel impactor against the ends of the vial to pulverize the brittle material. Researchers at Los Alamos National Laboratory (LANL) developed a method of cryogenic grinding of samples to homogenize them and allow the acquisition of a representative aliquant of the materials (LANL, 1996).

When samples agglomerate or “cake” during grinding, further particle size reduction is suppressed. Caking can be caused from moisture, heat, static charge accumulation, the fusing of particles under pressure, etc. When it occurs, caking is a serious challenge. There are two main approaches to this problem, slurry grinding and dry grinding.

- In slurry grinding, particles are suspended in solution during grinding. Water, alcohol, or other liquids are added to the sample before grinding, and have to be removed afterwards. Slurry grinding is a fairly reliable way of grinding a sample to micron-sized particles, but it is sloppy and time-consuming.

- Dry grinding is often simpler and quicker, but requires careful matching of the technique to the sample. If caking is due to moisture, as in many soils or cements, the sample should be dried before grinding. Grinding aids such as lubricants, antistatic agents, abrasives, and binding agents can also be used. Examples of grinding aids include dry soap or detergent (a lubricant), graphite (an antistatic agent as well as a lubricant), polyvinyl alcohol, phenyl acetate, propylene glycol, and aspirin. For example, propylene glycol (one drop for up to ten grams of sample) is used for laboratory fine grinding of Portland cement and many minerals.

Grinding efficiency can be improved through intermittent screening of the material. The ground sample is placed upon a wire or cloth sieve that passes particles of the desired size. The residual particles are reground and this process is repeated until the entire sample passes through the screen. Sieves with large openings can be used in the initial stages of sample preparation to remove unwanted large rocks, sticks, etc.

### **12.3.2 Soil/Sediment Samples**

For many studies, the majority of the solid samples will be soil/sediment samples or samples that contain some soil. The definition of soil is given in Chapter 10 (*Field and Sampling Issues that Affect Laboratory Measurements*). Size is used to distinguish between soils (consisting of sands, silts, and clays) and gravels.

The procedures to be followed to process a raw soil sample to obtain a representative subsample for analysis depend, to some extent, upon the size of the sample, the amount of processing already undertaken in the field, and more importantly, the radionuclide of interest and the nature of the contamination. Global fallout is relatively homogeneous in particle size and distribution in the sample, and therefore, standard preparation procedures should be adequate for this application. However, when sampling accidental or operational releases, the standard procedures may be inadequate. Transuranic elements, especially plutonium, are notorious for being present as “hot-spots” ions (Eberhardt and Gilbert, 1980; Sill, 1975) and great care must be employed so that the subsample taken for analysis accurately represents the total sample. This will depend on the size and the degree of homogeneity. Multiple subsampling, larger aliquants, and multiple analysis may be the only techniques available to adequately define the content of radionuclides in

heterogeneous samples. Therefore, it is imperative that the analyst choose a preparation approach appropriate to the nature of the sample.

#### 12.3.2.1 Soils

ASTM has developed a Standard Practice for the preparation of soil samples (ASTM C999). Guidance is given in this ASTM method for the preparation of a homogenous soil sample from composited core samples. The soil samples are dried at 110° C until at constant weight, ground and mixed in a ball mill, and processed through a U.S. Series No. 35 (500-µm or 32-mesh) sieve. This method is intended to produce a homogeneous sample from which a relatively small aliquant (10 g) may be drawn for radiochemical analyses.

A similar procedure for homogenizing soil samples is given in HASL-300 (DOE, 1997). Unwanted material (e.g, vegetation, large rocks) is removed as warranted, and the sample is dried. If the sample contains small rocks or pebbles, the entire soil sample is crushed to 6.35 mm, or the entire sample is sieved through a 12.7-mm screen. The sample is blended, then reduced in size by quartering. This subsample of soil is processed through a grinder, ball mill, sieve, or pulverizer until the soil is reduced to <1.3 mm (15 mesh equivalent).

Sill et al. (1974) described a procedure where they dried raw soil samples for two to three hours at 120° C and then ground the cooled sample lightly in a mortar and pestle. All rocks larger than ¼ inch were removed. The sample was charred at 400° C for two to three hours, cooled and passed though a No. 35 U.S. standard sieve, and then blended prior to aliquanting (10.0 g are taken for the analysis).

#### 12.3.2.2 Sediments

ASTM D3976 is a standard practice for the preparation of sediment samples for chemical analysis. This ASTM practice describes the preparation of test samples collected from streams, rivers, ponds, lakes, and oceans. The procedures are applicable to the determination of volatile, semivolatile, and nonvolatile constituents of sediments. Samples are first screened to remove foreign objects and then mixed by stirring. The solids are allowed to settle and the supernatant liquid is decanted. To minimize stratification effects due to differential rates of settling, the sample is mixed again before aliquanting for drying and analysis.

### **12.3.3 Biota Samples**

#### **12.3.3.1 Biological Samples**

ASTM D4638 is a standard guide for the preparation of biological samples for inorganic chemical analysis. This ASTM guide gives procedures for the preparation of test samples of plankton, mollusks, fish, and plants. The preparation techniques are applicable for the determination of volatile, semivolatile, and nonvolatile inorganic compounds in biological materials. However, different preparation steps are involved for the three classes of inorganic compounds. In the case of nonvolatile compounds, the first step is to remove foreign objects and most of the occluded water. For large samples such as fish, samples are homogenized using a tissue disrupter, blender, or equivalent, and a moisture determination is performed on a one to two gram aliquant. The samples then are dried by heating in an oven, by dessication, by air drying, by freeze drying, or by low-temperature drying using an infrared lamp, hot plate, or a low setting on a muffle furnace. Finally, the samples are dry ashed.

#### **12.3.3.2 Food**

The International Atomic Energy Agency has provided a guidebook for the measurement of radionuclides in food and the environment (IAEA, 1989). Sample preparations for milk and other foods such as meat, fish, fruit, vegetables, and grains are given in this guidebook. Additionally, methods are presented in HASL-300 for the preparation of milk, vegetables, composite diets, etc. These methods generally involve dry ashing. The samples first are dried thoroughly at 125° C. Then, the temperature is raised at intervals over an 8-hour period through the critical range where ignition occurs, and finally to 500° C for 16 hours. If only a portion of ash is to be used for analysis, it is ground and sieved prior to aliquanting.

#### **12.3.3.3 Vegetation**

There are several DOE site references that contain examples of sample preparation for vegetation. Los Alamos National Laboratory (LANL, 1997) recently grew pinto beans, sweet corn, and zucchini squash in a field experiment at a site that contained observable levels of surface gross gamma radioactivity within Los Alamos Canyon. Washed edible and nonedible crop tissues (as well as the soil) were prepared for analysis for various radionuclides. Brookhaven National Laboratory has also evaluated the effect of its operation on the local environment. Their site environmental report (DOE, 1995) gives sample preparation steps for radionuclide analysis of vegetation and fauna (along with ambient air, soil, sewage effluent,



surface water, and groundwater). HASL-300 also describes sample preparation techniques for vegetation samples for a variety of radionuclides.

#### 12.3.3.4 Bone and Tissue

Bone and tissue samples can be dry ashed in a muffle furnace (HASL-300, Fisenne, 1994; Fisenne et al., 1980), wet ashed with nitric acid and peroxide (Fisenne and Perry, 1978) or alternately dry ashed and wet ashed with nitric acid until all visible signs of carbonaceous material has disappeared (McInroy et al., 1985).

#### 12.3.4 Other Samples

The category “other” includes such matrices as concrete, asphalt, coal, plastic, etc. The sample preparation procedures applied to soils are generally applicable for the “other” category, except for more aggressive grinding and blending in the initial step. For example, items such as plastic or rubber which are too flexible to be impact-ground at room temperature must be ground cryogenically. They are embrittled by chilling and then pulverized. ASTM C114 describes the sample preparation steps for the chemical analysis of hydraulic cement, whereas ASTM C702 describes the sample preparation of aggregate samples, and is also applicable to lime and limestone products as noted in ASTM C50. Additionally, ASTM D2013 describes the preparation of coal samples for analysis.

### 12.4 Filters

Filters are used to collect analytes of interest from large volumes of liquids or gases. The exact form of the filter depends on the media (e.g., air, aqueous liquid, nonaqueous liquid), the analyte matrix (e.g., sediment, suspended particulates, radon gas), and the objectives of the project (e.g., volume of sample passing through the filter, flow rate through the filter, detection limits, etc. (see the section on filtration in Chapter 10, *Field and Sampling Issues that Affect Laboratory Measurements*).

**TABLE 12.4—Preliminary Ashing Temperature for Food Samples**

(Method Sr-02-RC, HASL-300 [DOE, 1997])

Material	Temperature (° C)
Eggs . . . . .	150-250
Meat . . . . .	Burning
Fish . . . . .	Burning
Fruit (fresh) . . . . .	175-325
Fruit (canned) . . . . .	175-325
Milk (dry) . . . . .	—
Milk (wet) . . . . .	175-325
Buttermilk (dry) . . . . .	—
Vegetables (fresh) . . . . .	175-225
Vegetables (canned) . . . . .	175-250
Root vegetables . . . . .	200-325
Grass . . . . .	225-250
Flour . . . . .	Burning
Dry beans . . . . .	175-250
Fruit juices . . . . .	175-225
Grains . . . . .	225-325
Macaroni . . . . .	225-325
Bread . . . . .	225-325

Filter samples from liquids usually consist of the filter with the associated solid material. For samples with a large amount of sediment, the solid material may be removed from the filter and analyzed as a solid. When there is a relatively small amount of solid material, the filter may be considered as part of the sample for analytical purposes. When large volumes of liquid are processed at high flow rates, filter cartridges often are used. Typically, the cartridge case is not considered part of the sample, and laboratory sample preparation includes removing the filter material and sample from the cartridge case. Any special handling instructions should be included as SOPs in the planning documents.

Air filters may be particulate filters, which are prepared in the same manner as liquid filters, or they may be cartridges of absorbent material. Filters that absorb materials are typically designed for a specific analysis. For example, activated charcoal cartridges are often used to collect samples of iodine or radon. Silver zeolite cartridges may be used for noble gases such as argon, krypton, or xenon. These cartridges are often designed to be analyzed intact, so no special sample preparation is needed. If the cartridges need to be disassembled for analysis, a special SOP for preparing these samples is usually required.

Homogenization is rarely an issue when preparing filter samples. Typically, the entire filter is digested and analyzed. However, obtaining a representative sample of a filter does become an issue when the entire filter is not analyzed. The planning document should give the details of sample preparation for portions of a filter (e.g., sample size reduction through quartering). Steps such as using tweezers for holding filters and using individual sample bags should be taken to prevent the loss of material collected on the filter during handling and processing.

## **12.5 Wipe Samples**

Wipe samples (also referred to as “swipes” or “smears”) are collected to indicate the presence of removable surface contamination. The loose contamination is transferred from the surface to a sample of wipe material. The wipe material can be virtually anything, but common materials include Whatman filter paper and nylon membrane. The greatest challenge in preparing wipe samples is homogenizing the sample to obtain a representative portion for analysis, although usually the entire wipe is analyzed. Wipe samples are commonly digested prior to analysis, but they can be analyzed directly through appropriate counting techniques (McFarland, 1998a, 1998b).

Many wipe samples are collected using filter paper or disc smears. In many cases, the contamination on these samples is simply assumed to be fairly evenly distributed, and the wipe samples are prepared like filter samples. Sometimes, a specific analytical procedure is anticipated

and a special wipe material is used. For example, Styrofoam generates static electricity and can attract dust particles from a relatively clean surface. Styrofoam is dissolved easily in most (if not all) commercially available liquid scintillation cocktails. These wipe samples can be very easily collected, stored, and transported in liquid scintillation vials. Have the cocktail added by the laboratory and be counted for gross alpha and gross beta activity using a liquid scintillation counter.

## **12.6 Liquid Samples**

Liquid samples are commonly classified as aqueous, nonaqueous, and mixtures. Aqueous liquids are most often surface water, groundwater, drinking water, precipitation, effluent, or runoff. Nonaqueous liquids may include solvents, oils, or other organic liquids. Mixtures may be combinations of aqueous and nonaqueous liquids, but may include solid material mixed with aqueous or nonaqueous liquids or both.

Preliminary sample measurements (e.g., conductivity, turbidity) may be performed to provide information about the sample and to confirm field processing (see measurement of pH to confirm field preservation in Chapter 11). These measurements are especially useful when there is no prior historical information available from the sample collection site. In addition, this information can also be helpful in the performance of certain radiochemical analyses. These preliminary measurements typically require little or no sample preparation. In many cases, the results of preliminary measurements can be used to determine the quantity of sample to be used for a specific analysis.

### **12.6.1 Conductivity**

In radiochemistry, conductivity measurements typically are used as a surrogate to estimate dissolved solids content for gross-alpha and gross-beta measurements. Because the preservation of samples with acid prevents the measurement of conductivity, the recommendation is to perform the QC checks for conductivity in the field when the original measurements are performed. If the sample is not preserved in the field, the measurement can be done in the laboratory.

ASTM D1125 is the standard test method for determining the electrical conductivity of water. The method is used for the measurement of ionic constituents, including dissolved electrolytes in natural and treated water.

### **12.6.2 Turbidity**

The presence of dissolved or suspended solids, liquids, or gases causes turbidity in water. Measurement of turbidity provides a means to determine if removal of suspended matter is necessary in order to meet the specifications for liquid samples as given in the plan document. ASTM D1889 is the standard test method for the determination of turbidity of water and wastewater in the range from 0.05 to 40 nephelometric turbidity units (NTU). In the ASTM method, a photoelectric nephelometer is used to measure the amount of light that a sample scatters when the light is transmitted through the sample.

### **12.6.3 Filtration**

The filtration of samples is based on the appropriate plan document which should also give the selection of the filter material to be used. If samples have not been filtered in the field, the laboratory can perform the filtration. Guidance on filtration of liquid samples is provided in Section 10.3.3. Filtering is normally done in the field so that preservatives can be added without promoting the dissolution of undissolved solids in the sample at the time of collection.

### **12.6.4 Aqueous Liquids**

Aqueous liquids are a common matrix analyzed by laboratories, and are often referred to as *water samples*. Examples of possible aqueous liquids requiring radionuclide analysis include the following:

- Drinking water;
- Surface water;
- Ground water;
- Soil pore water;
- Storage tank water;
- Oil production water or brine;
- Trench or landfill leachate; and
- Water from vegetation.

For certain samples that are not filtered, inversion is a form of homogenization. Typically, the sample is homogenized by inverting the container several times to mix the sample thoroughly. If there is some air in the container, the passage of air bubbles through the sample will create sufficient turbulence to mix the sample thoroughly with three or four inversions of the sample container. If the sample contains zero headspace (so there is no air in the sample container), the

sample should be inverted and allowed to stay inverted for several seconds before the next inversion. Ten to twenty inversions of the sample container may be required to ensure that the sample is mixed thoroughly under zero headspace conditions. Simply shaking the container will not mix the contents as thoroughly as inverting the sample container. Mechanical shakers, mixers, or rotators may be used to homogenize aqueous samples thoroughly.

Filtration and acidification performed in the field is typically the only preparation required for aqueous liquids (Chapter 10). A general discussion concerning preparation of water samples for the measurement of radioactivity is presented in NCRP (1976). *Analytical Chemistry Laboratory Sample Preparation Methods* (ACL, 1992) gives a number of sample preparation methods for various materials, including water samples.

ASTM gives standard test methods for the preparation of water samples for the determination of alpha and beta radioactivity (ASTM D1943 and D1890, respectively). After collecting the water sample in accordance with ASTM D3370, the sample is made *radioactively homogeneous* by addition of a reagent in which the radionuclides present in the sample are soluble in large concentrations. Acids, complexing agents, or chemically similar stable carriers may be used to obtain homogeneity. The chemical nature of the radionuclides and compounds present and the subsequent steps in the method will indicate the action to be taken. Different preparation techniques for freshwater and seawater samples are illustrated in *Radiochemical Analytical Procedures for Analysis of Environmental Samples* (EPA, 1979) and for drinking water in EPA (1980).

#### 12.6.5 Nonaqueous Liquids

Nonaqueous liquids can be substances other than water such as organic solvents, oil, or grease. Many organic solvents are widely used to clean oil, grease, and residual material from electrical and mechanical equipment. The resulting waste liquid may contain a significant amount of solid material. It may be necessary to filter such liquids to determine (1) if the analyte is contained in the filtrate and is soluble, or (2) if the analyte is contained in the solids and therefore is insoluble. The appropriate plan document should be reviewed to determine if filtration is necessary. ASTM C1234, Standard Test Method for *Preparation of Oils and Oily Waste Samples by High-Pressure, High-Temperature Digestion for Trace Element Determinations*, describes the preparation of homogeneous samples from nuclear processing facilities.

Homogenization of nonaqueous samples is accomplished in a manner similar to that for aqueous samples. Visual inspection is typically used as a qualitative measure of homogeneity in nonaqueous samples. If a quantitative measure of mixing is desired, turbidity measurements can

be performed after a predetermined amount of mixing (e.g., every 10 inversions, every 2 minutes, etc.) until a steady level of turbidity is achieved (e.g., 1 to 10 percent variance, depending on the project objectives—see ASTM D1889, *Standard Test Method for Turbidity of Water*).

DOE (ANL/ACL, 1995) evaluated sample preparation techniques used for the analysis of oils. In evaluating the performance of a sample preparation technique, DOE considered the following qualities to be important:

- Thorough sample decomposition;
- Retention of volatile analytes;
- Acceptable analyte recovery;
- Minimal contamination from the environment or the digestion vessel;
- Low reagent blanks; and
- Speed.

One of the preparation methods involved combustion of oil under oxygen at 25 atm pressure (ASTM E926) and another used nitric acid decomposition of the oil in a sealed vessel heated with a microwave (EPA, 1990).

Many nonaqueous liquids present a health hazard (e.g., carcinogenicity) or require special safety considerations (e.g., flammability). Any special handling requirements based on health and safety considerations should be documented in the planning documents.

## **12.6.6 Mixtures**

Some common examples of mixtures that may be encountered by the laboratory are water with lots of total dissolved solids and undissolved solids or water and oil in separate layers. The following sections discuss preparation procedures for these types of mixtures.

### **12.6.6.1 Liquid-Liquid Mixtures**

When aqueous and nonaqueous liquids are combined, they usually form an immiscible mixture, such as oil and water.<sup>1</sup> In most cases, a separatory funnel helps in separating the liquids into two

---

<sup>1</sup> It is often necessary to determine which liquid is aqueous and which liquid is nonaqueous. Never assume that the top layer is always nonaqueous, or the bottom layer is always aqueous. The density of the bottom layer is always greater than the density of the top layer. Halogenated solvents (e.g., carbon tetrachloride, CCl<sub>4</sub>) tend to have  
(continued...)

1098 samples. Each sample then is analyzed separately. If, in the rare case, both liquids must be  
1099 processed together, there is greater difficulty in preparing the combined liquids for analysis.  
1100 Obtaining a homogenous aliquant is a key consideration in this case. Often times, the entire  
1101 sample should be analyzed. This approach avoids processing problems and yields the desired  
1102 result.

#### 1103 12.6.6.2 Liquid-Solid Mixtures

1104 Mixtures of liquids and solids are usually separated by filtering, centrifuging, or decanting, and  
1105 the two phases are analyzed separately. If the mixture is an aqueous liquid and a solid, and will  
1106 be analyzed as a single sample, the sample is often treated as a solid. Completely drying the  
1107 sample followed by dry ashing before any attempt at wet ashing is recommended to reduce the  
1108 chance of organic solids reacting with strong oxidizing acids (e.g.,  $\text{H}_2\text{SO}_4$ ,  $\text{HNO}_3$ , etc.). If the  
1109 mixture includes a nonaqueous liquid and a solid, it is suggested that the phases be separated by  
1110 filtration and the solid rinsed thoroughly with a volatile solvent such as ethanol or methanol  
1111 before continuing with the sample preparation process.

1112 In rare cases where a sample contains a mixture of aqueous liquid, nonaqueous liquid, and solid  
1113 material, the sample can be separated into three different phases before analysis. The sample  
1114 should be allowed to settle overnight and the liquids decanted. The liquids can then be separated  
1115 in a separatory funnel without the solid material clogging the funnel. Each liquid should be  
1116 filtered to remove any remaining solid material. The solid should be filtered to remove any  
1117 remaining liquid and rinsed with a volatile solvent. This rinse removes any traces of organic  
1118 liquids to reduce problems during subsequent dissolution activities. The three phases are then  
1119 analyzed separately. If necessary, the results can be added together to obtain a single result for the  
1120 mixture after the separate analyses are completed.

### 1121 12.7 Gases

1122 Sample preparation steps are usually not required for gas samples. Lodge (1988) gives general  
1123 techniques, including any necessary sample preparation, for the sampling and storage of gases

---

<sup>1</sup>(...continued)

densities greater than about 1 g/mL, so they typically represent the bottom layer. Other organic liquids (e.g., diethyl ether, oil, etc.) tend to have densities less than 1 g/mL, so they typically represent the top layer. Mixtures of organic liquids may have almost any density. To test the liquids, add a drop of water to the top layer. If the drop dissolves in the top layer, the top layer is aqueous. If the drop settles through the top layer and dissolves in the bottom layer, the bottom layer is aqueous.

and vapors. The determination of the tritium content of water vapor in the atmosphere is one of the example procedures. ASTM D3442 is a standard test method for the measurement of total tritium activity in the atmosphere. Sample preparation is covered in this test method.

EPA has prepared “Background Information Document: Procedures Approved for Demonstrating Compliance with 40 CFR Part 61” (EPA, 1989) for use in demonstrating compliance with the radionuclide National Emission Standards for Hazardous Air Pollutants (NESHAP). This document includes references to air sampling and sample preparation. Table 3-1 of EPA (1989) lists numerous references to radionuclide air sampling and preparation; examples include:

- *A Study of Airborne Radioactive Effluents from the Pharmaceutical Industry* (Cehn, 1979).
- “The Fraction of Material Released as Airborne Activity During Typical Radioiodinations,” (Eichling, 1983).
- “Application for Renewal of Source Material License: SUB-526, Docket 40-3392,” (Allied Chemical, 1982).
- “Airborne Concentrations of I-131 in a Nuclear Medicine Laboratory” (Browning et al., 1978).

## **12.8 Bioassay**

Analyses of bioassay samples are necessary to monitor the health of employees involved in radiological assessment work. Normally these types of samples include urine and fecal specimens.

Urine samples are typically wet ashed with nitric acid (DOE, 1997; HASL-300) or with nitric acid and peroxide (RESL, 1982). Alternatively, there are procedures which co-precipitate the target analytes in urine by phosphate precipitation (Horwitz et al., 1990; Stradling and Popplewell, 1974; Elias, 1997). Fecal samples are normally dry ashed in a muffle furnace (HASL-300), or prepared by lyophilization, “freeze drying” (Dugan and McKibbin, 1993).

It is important to note that although ANSI 13.30 indicates that aliquanting a homogeneous sample to determine the activity present in the total sample is acceptable, this standard dictates that the entire sample should be prepared for analysis and the aliquant taken after the sample preparation has been completed.



## 12.9 References

### 12.9.1 Cited Sources

Allied Chemical UF<sub>6</sub> Conversion Plant. 1982. "Application for Renewal of Source Material License: SUB-526, Docket 40-3392," Metropolis, Illinois.

American National Standards Institute (ANSI). 1996. ANSI 13.30 *Performance Criteria for Radiobioassay*. Health Physics Society.

Analytical Chemistry Laboratory (ACL) Procedure Compendium. 1992. *Volume 2: Sample Preparation Methods*. Battelle Pacific Northwest Laboratories, PNL-MA-559.

ANL/ACL. 1992. *Innovative Methods for Inorganic Sample Preparation*. Argonne National Laboratory, April 1992.

ANL/ACL. 1995. *Preparation of Waste Oil for Analysis to Determine Hazardous Metals*. Argonne National Laboratory, July.

Association of Official Analytical Chemists International (AOAC). 1995. Official Method 985.14. "Moisture in Meat and Poultry Products," in *Official Methods of Analysis of AOAC International*; Cuniff, P., Ed., Arlington, VA.

Association of Official Analytical Chemists International (AOAC). 1995. Official Method 985.26. "Solids (Total) in Processed Tomato Products", In *Official Methods of Analysis of AOAC International*; Cuniff, P., Ed.; Association of Official Analytical Chemists International: Arlington, VA.

American Society for Testing and Materials (ASTM) C50. Standard Practice for *Sampling, Inspection, Packing, and Marking of Lime and Limestone Products*.

American Society for Testing and Materials (ASTM) C114. Standard Test Method for *Chemical Analysis of Hydraulic Cement*.

American Society for Testing and Materials (ASTM) C702. Standard Practice for Reducing Samples of Aggregate to Testing Size, Vol 04.02.

## *Laboratory Sample Preparation*

---

- 1177 American Society for Testing and Materials (ASTM) C999. Standard Practice for *Soil Sample*  
1178 *Preparation for the Determination of Radionuclides.*
- 1179 American Society for Testing and Materials (ASTM) C1234. Standard Test Method for  
1180 *Preparation of Oils and Oily Waste Samples by High-Pressure, High-Temperature Digestion*  
1181 *for Trace Element Determinations.*
- 1182 American Society for Testing and Materials (ASTM) D1125. Standard Test Method for  
1183 *Determining the Electrical Conductivity of Water.*
- 1184 American Society for Testing and Materials (ASTM) D1889. Standard Test Method for *Turbidity*  
1185 *of Water.*
- 1186 American Society for Testing and Materials (ASTM) D1890. Standard Test Method for *Beta*  
1187 *Particle Radioactivity of Water.*
- 1188 American Society for Testing and Materials (ASTM) D1943. Standard Test Method for *Alpha*  
1189 *Particle Radioactivity of Water.*
- 1190 American Society for Testing and Materials (ASTM) D2013. Standard Method of *Preparing*  
1191 *Coal Samples for Analysis.*
- 1192 American Society for Testing and Materials (ASTM) D3370. Standard Practices for *Sampling*  
1193 *Water from Closed Conduits.*
- 1194 American Society for Testing and Materials (ASTM) D3442. Standard Test Method for *Gaseous*  
1195 *Tritium Content of the Atmosphere.*
- 1196 American Society for Testing and Materials (ASTM) D3974. Standard Practice for *Extraction of*  
1197 *Trace Elements from Sediments.*
- 1198 American Society for Testing and Materials (ASTM) D3975, Standard Practice for *Development*  
1199 *and Use (Preparation) of Samples for Collaborative Testing of Methods for Analysis of*  
1200 *Sediments.*
- 1201 American Society for Testing and Materials (ASTM) D3976. Standard Practice for *Preparation*  
1202 *of Sediment Samples for Chemical Analysis.*

- 1203 American Society for Testing and Materials (ASTM) D4638. Standard Guide for *Preparation of*  
1204 *Biological Samples for Inorganic Chemical Analysis*.
- 1205 American Society for Testing and Materials (ASTM) D4643. Standard Test Method for  
1206 *Determination of Water (Moisture) Content in Soil by the Microwave Oven Method*.
- 1207 American Society for Testing and Materials (ASTM) E926. Standard Practices for *Preparing*  
1208 *Refuse-Derived Fuel (RDF) Samples for Analyses of Metals*.
- 1209 American Society for Testing and Materials (ASTM) E1358. Standard Test Method for  
1210 *Determination of Moisture Content of Particulate Wood Fuels Using a Microwave Oven*.
- 1211 Beary, E.S. 1988. "Comparison of Microwave Drying And Conventional Drying Techniques For  
1212 Reference Materials." *Anal. Chem* Vol. 60, pp. 742-746.
- 1213 Bernabee, R. P., D. R. Percival, and D. B. Martin. 1980. "Fractionation of Radionuclides in  
1214 Liquid Samples from Nuclear Power Facilities." *Health Physics* Vol. 39, pp. 57-67.
- 1215 Bock, R. 1979. *A Handbook of Decomposition Methods in Analytical Chemistry*. International  
1216 Textbook Company, Limited. T. & A. Constable Ltd., Great Britain.
- 1217 Browning, E.J., K. Banerjee, and W.E. Reisinger. 1978. "Airborne Concentrations of I-131 in a  
1218 Nuclear Medicine Laboratory," *Journal of Nuclear Medicine*, Vol. 19, pp. 1078-1081.
- 1219 Cameron, P., and Murgatroyd, K. 1996. *Good Pharmaceutical Freeze-Drying Practice*.  
1220 Interpharm Press.
- 1221 Cehn, J.I. 1979. *A Study of Airborne Radioactive Effluents from the Pharmaceutical Industry*,  
1222 Final Report, Prepared by Teknekron, Inc., for the U.S. EPA Eastern Environmental Research  
1223 Facility, Montgomery, AL.
- 1224 Dean, J.A. 1995. *Analytical Chemistry Handbook*, McGraw-Hill, Inc., New York.
- 1225 DeVoe, J.R. 1961. *Radioactive Contamination of Materials Used in Scientific Research*.  
1226 Publication 895, NAS-NRC.
- 1227 Dugan, J.P. and T.T. McKibbin. 1993. "Preparation of Fecal Samples for Radiobioassay by  
1228 Lyophilization," *Radioactivity & Radiochemistry* 4:3, pp. 12-15.

- 1229 Eberhardt, L.L., and R.O. Gilbert. 1980. "Statistics and Sampling in Transuranic Studies," in  
1230 Transuranic Elements in the Environment , edited by W.C. Hanson, U.S. Department of  
1231 Energy. DOE/TIC-22800.
- 1232 Eichling, J. 1983. "The Fraction of Material Released as Airborne Activity During Typical  
1233 Radioiodinations," Proceedings of the 9<sup>th</sup> Biennial Conference of Campus Radiation Safety  
1234 Officers, University of Missouri-Columbia, June 6-8, 1983.
- 1235 Elias, G. 1997. "A Rapid Method for the Analysis of Plutonium and Uranium in Urine Samples,"  
1236 *Radioactivity & Radiochemistry* 8:3, pp. 20-24.
- 1237 Fisenne, I.M. and P. Perry 1978. "The Determination of Plutonium in Tissue by Aliquat-336  
1238 Extraction," *Radiochem Radioanal. Letters* Vol. 33, pp. 259-264.
- 1239 Fisenne, I.M., P. Perry and G.A. Welford. 1980. "Determination of Uranium Isotopes in Human  
1240 Bone Ash," *Anal. Chem.* Vol. 52, pp. 777-779.
- 1241 Fisenne, I.M. 1994. "Lead-210 in Animal and Human Bone: A New Analytical Method," *Env.*  
1242 *Int.* Vol. 20, pp. 627-632.
- 1243 Greenberg, A.E., L.S. Clesceri, and A.D. Eaton (Eds). 1992. *Standard Methods for the*  
1244 *Examination of Water and Wastewater*. American Public Health Association.
- 1245 Greenwood, N. N. and A. Earnshaw. 1984. *Chemistry of the Elements*. Pergamon Press, Inc.  
1246 Elmsford, New York.
- 1247 Gy, Pierre M. 1992. *Sampling of Heterogeneous and Dynamic Material Systems: Theories of*  
1248 *Heterogeneity, Sampling, and Homogenizing*. Elsevier, Amsterdam, The Netherlands.
- 1249 Horwitz, E.P., M.L. Dietz, D.M. Nelson, J.J. LaRosa, and W.D. Fairman 1990. "Concentration  
1250 and Separation of Actinides from Urine using a Supported Bifunctional Organophosphorous  
1251 Extractant," *Analytica Chimica Acta*. Vol. 238, pp. 263-271.
- 1252 IAEA. 1989. *Measurement of Radionuclides in Food and the Environment—A Guidebook*.  
1253 Technical Reports Series No. 295, International Atomic Energy Agency, Vienna.
- 1254 Kingston, H.M., and Jassie, L.B. 1988. *Introduction to Microwave Sample Preparation: Theory*  
1255 *and Practice*, American Chemical Society, Washington, DC.

- 1256 Koh, T.S. 1980. *Anal Chem* Vol. 52, pp. 1978-1979.
- 1257 Kralian, M.A., M.J. Atkins, and S.A. Farber. 1990. "Guidelines for Effective Low-Level  
1258 Contamination Control in a Combination Environmental/Radioactive Waste Analysis  
1259 Facility," *Radioactivity & Radiochemistry*. 1:3, pp. 8-18.
- 1260 Lodge, J. 1988. *Methods of Air Sampling and Analysis*. Third Edition, CRC Press, Florida.
- 1261 LANL. 1996. *Application of Cryogenic Grinding to Achieve Homogenization of Transuranic*  
1262 *Waste*, Atkins, W. H., LANL-13175.
- 1263 Los Alamos National Laboratory (LANL). 1997. *Radionuclide Concentration in pinto beans,*  
1264 *sweet corn, and zucchini squash grown in Los Alamos Canyon at Los Alamos National*  
1265 *Laboratory*, Fresquez, P. R., M. A. Mullen, L. Naranjo, and D. R. Armstrong, May 1997.
- 1266 Lucas, H.F., Jr. 1963. "A Fast and Accurate Survey Technique for Both Radon-222 and Radium-  
1267 226," *The Natural Radiation Environment, Proceedings of the International Symposium,*  
1268 *William Rice University, Houston, TX, 315-319.*
- 1269 Lucas, H.F. 1967. "A Radon Removal System for the NASA Lunar Sample Laboratory: Design  
1270 and Discussion," Argonne National Laboratory Radiological Physics Division Annual  
1271 Report, ANL-7360.
- 1272 McFarland, R.C. 1998a. "Determination of Alpha-Particle Counting Efficiency for Wipe-Test  
1273 Samples," *Radioactivity & Radiochemistry*. 9:1, pp. 4-8.
- 1274 McFarland, R.C. 1998b. "Determination of Counting Efficiency for Wipe-Test Samples  
1275 Containing Radionuclides that Emit High-Energy Beta Particles," *Radioactivity &*  
1276 *Radiochemistry* 9:1, pp. 4-9.
- 1277 McInroy, J.F., H.A. Boyd, B.C. Eutsler, and D. Romero. 1985. "Part IV: Preparation and  
1278 Analysis of the Tissue and Bones," *Health Physics*, 49:4, pp. 585-621.
- 1279 NCRP Report No. 50. 1976. *Environmental Radiation Measurements*.
- 1280 Obenhaus, R.H., R. Bostwick, W. Fithian, M. McCann, J.D. McCormack, and D. Selem *SPEX*  
1281 *CertiPrep Handbook of Sample Preparation and Handling*, SPEX CertiPrep, Inc., Metuchen,  
1282 NJ. Also, at <http://www.spexcsp.com/spmain>.

*Laboratory Sample Preparation*

---

- 1283 Pitard, F. F. 1993. *Pierre Gy's Sampling Theory and Practice*. CRC Press, Inc., Boca Raton, FL.  
1284 Second Edition.
- 1285 RESL Analytical Chemistry Branch Procedures Manual, DOE-ID, collected and published in  
1286 1982 and containing procedures beginning in 1969.
- 1287 Schilt, A. 1979. *Perchloric Acid and Perchlorates*. The G. Frederick Smith Chemical Company,  
1288 Columbus, Ohio.
- 1289 Scwedt, G. 1997. *The Essential Guide to Analytical Chemistry* (Translation of the revised and  
1290 updated German Second Edition. Translated by Brooks Haderlie), John Wiley & Sons,  
1291 England.
- 1292 Sedlet, J. 1966. "Radon and Radium," in *Treatise on Analytical Chemistry*, Part II, Vol. IV,  
1293 p219-366, edited by I.M. Kolthoff and P.J. Elving, John Wiley & Sons, Inc, New York.
- 1294 Shugar, G.J. and J.T. Ballinger. 1996. *Chemical Technicians' Ready Reference Handbook*.  
1295 McGraw-Hill, New York.
- 1296 Sill, C.W., K.W. Puphal, and F.D. Hindman. 1974. "Simultaneous Determination of Alpha-  
1297 Emitting Nuclides of Radium through Californium in Soil," *Anal. Chem* 46:12, pp. 1725-  
1298 1737.
- 1299 Sill, C.W. 1975. "Some Problems in Measuring Plutonium in the Environment," *Health Physics*.  
1300 Vol. 29, pp. 619-626.
- 1301 Stradling, G.N. and D.S. Popplewell. 1974. "Rapid Determination of Plutonium in Urine by  
1302 Ultrafiltration," *Int. J. Appl. Radiation Isotopes*. Vol. 25, p 217.
- 1303 U.S. Department of Energy (DOE). 1990. *EML Procedures Manual* (HASL-300-Ed.27), G. de  
1304 Planque, Environmental Measurements Laboratory.
- 1305 U.S. Department of Energy (DOE). 1995. *Brookhaven National Laboratory Site Environmental*  
1306 *Report for Calendar Year 1995*, Naidu, J. R., D. E. Paquette, G. L. Schroeder, BNL  
1307 December, 1996.
- 1308 U.S. Department of Energy. 1997 (DOE). *EML Procedures Manual* (HASL-300-Ed.28), Edited  
1309 by N.A. Chieco, Environmental Measurements Laboratory.

- 1310 U.S. Environmental Protection Agency (EPA). 1979. *Radiochemical Analytical Procedures for*  
 1311 *Analysis of Environmental Samples*; F. B. Johns, P. B. Hahn, D. J. Thome, and E. W.  
 1312 Bretthauer, EMSL, March 1979.
- 1313 U.S. Environmental Protection Agency (EPA). 1980. *Prescribed Procedures for Measurement of*  
 1314 *Radioactivity in Drinking Water*. H. L. Krieger and E. L. Whittaker, EPA 600-4-80-032,  
 1315 August 1980.
- 1316 U.S. Environmental Protection Agency (EPA). 1989. *Background Information Document:*  
 1317 *Procedures Approved for Demonstrating Compliance with 40 CFR Part 61, Subpart I*. EPA  
 1318 520-1-89-001, Office of Radiation Programs, October, 1989.
- 1319 U.S. Environmental Protection Agency (EPA). 1990. *Test Methods for Evaluating Solid Waste—*  
 1320 *Physical/Chemical Methods*. SW-846, Third Edition, Method 3051.
- 1321 U.S. Environmental Protection Agency (EPA). 1992. *Manual for the Certification of*  
 1322 *Laboratories Analyzing Drinking Water: Criteria and Procedures. Fourth Edition*, EPA 814-  
 1323 B-92-002, Office of Ground Water and Drinking Water, Cincinnati, Ohio.
- 1324 Walter, P., S. Chalk, and H. Kingston. 1997. “Overview of Microwave-Assisted Sample  
 1325 Preparation.” Chapter 2, *Microwave-Enhanced Chemistry*, H. Kingston and S. Haswell,  
 1326 editors, American Chemical Society, Washington, DC.
- 1327 Wang, C.H., Willis, D.L., and Loveland W.D. 1975. *Radiotracer Methodology in the Biological,*  
 1328 *Environmental, and Physical Sciences*. Prentice-Hall, Inc., New Jersey.
- 1329 Yamamoto, M., Komura, K., and Ueno, K. 1989. “Determination of Low-Level <sup>226</sup>Ra in  
 1330 Environmental Water Samples by Alpha-Ray Spectrometry,” *Radiochimica Acta* Vol. 46, pp.  
 1331 137-142.
- 1332 Zhang, H. and P. Dotson. 1998. *The Use of Microwave Muffle Furnace for Dry Ashing Plant*  
 1333 *Tissue Samples*. CEM Corporation. Also, *Commun. Soil Sci. Plant Anal.* 25:9&10, pp. 1321-  
 1334 1327 (1994).

## 1335 **12.9.2 Other Sources**

- 1336 American Society for Testing and Materials (ASTM) D5245. Standard Practice for *Cleaning*  
 1337 *Laboratory Glassware, Plasticware, and Equipment Used in Microbiological Analyses*.

*Laboratory Sample Preparation*

---

- 1338 American Society for Testing and Materials (ASTM) E1157. Standard Specification for  
1339 *Sampling and Testing of Reusable Laboratory Glassware*.
- 1340 Delherz, R. 1957. *Chemist-Analyst*. Vol. 46, p. 11.
- 1341 Kahn, B., Shleien, B., and Weaver, C. 1972. "Environmental Experience with Radioactive  
1342 Effluents From Operating Nuclear Power Plants," page 559 in *Peaceful Uses of Atomic*  
1343 *Energy*, Vol. 11 (United Nations, New York). Also, Kahn, B. 1973. "Determination of  
1344 Radioactive Nuclides in Water," page 1357 in *Water and Water Pollution Handbook*, Vol. 4  
1345 Ciaccio, L. L., Ed. (M. Decker, New York).
- 1346 Krieger, H.L. and E.L. Whittaker. 1980. "Prescribed Procedures for Measurement of  
1347 Radioactivity in Drinking Water," Environmental Monitoring and Support Laboratory,  
1348 Cincinnati, OH, EPA-600/4-80-032.
- 1349 Laug, E.P. 1934. *Ind. Eng. Chem., Anal Ed.* Vol. 13, pp. 419.
- 1350 Shugar and Dean. 1990. *The Chemist's Ready Reference Handbook*, McGraw-Hill.
- 1351 U.S. Environmental Protection Agency. 1987. *Eastern Environmental Radiation Facility*  
1352 *Radiochemistry Procedures Manual*. Compiled and edited by R. Lieberman, EPA 520-5-84-  
1353 006, Office of Radiation Programs, August, 1987.